
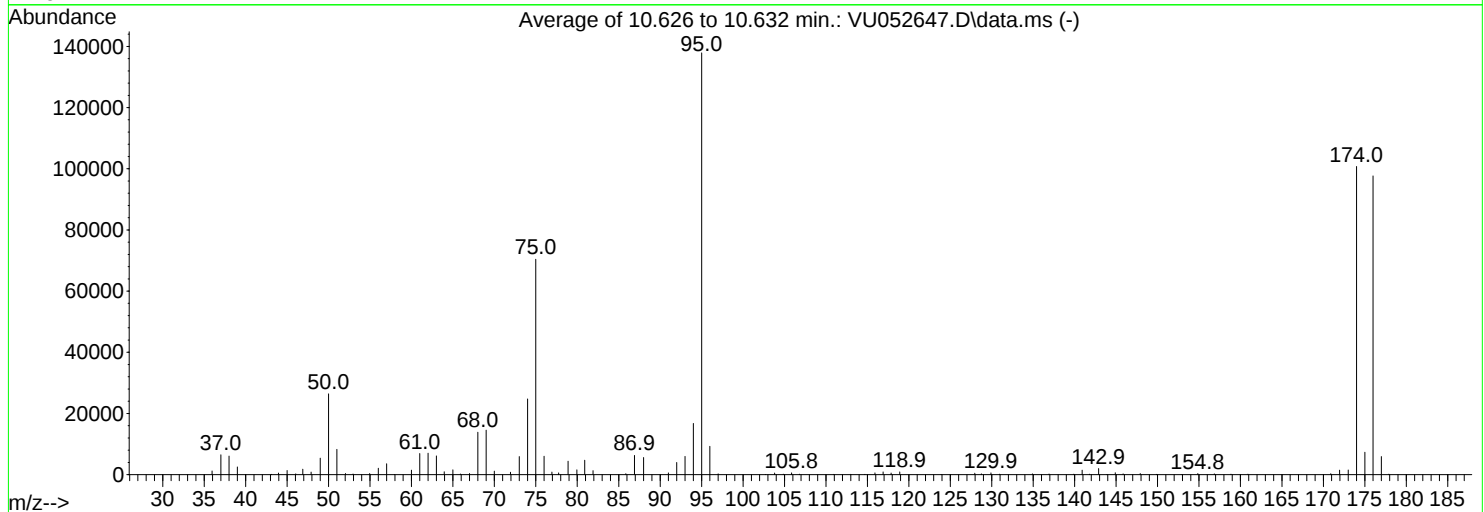


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU011123\  
Data File : VU052647.D  
Acq On : 11 Jan 2023 09:33  
Operator : JC/MD  
Sample : BFB  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U011123W.M  
Title : SW846 8260  
Last Update : Fri Jan 13 01:24:13 2023

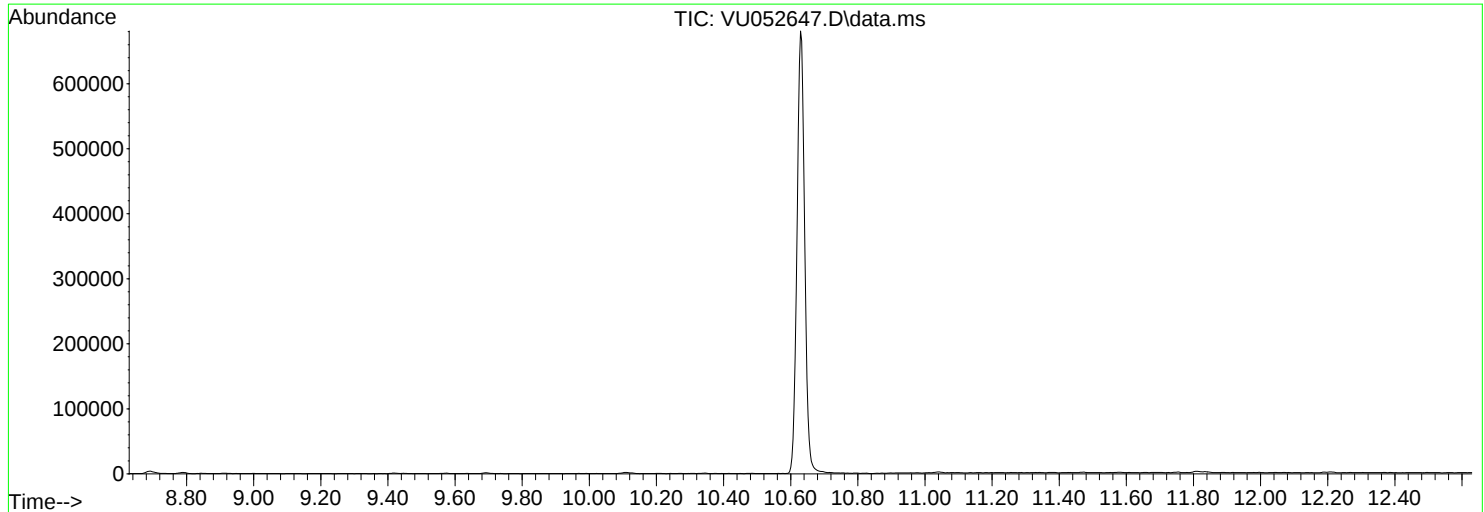

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 19.2         | 26416      | PASS                |
| 75             | 95              | 30              | 60              | 51.1         | 70435      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 137899     | PASS                |
| 96             | 95              | 5               | 9               | 6.7          | 9246       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.5          | 1517       | PASS                |
| 174            | 95              | 50              | 100             | 73.1         | 100760     | PASS                |
| 175            | 174             | 5               | 9               | 7.3          | 7326       | PASS                |
| 176            | 174             | 95              | 101             | 96.9         | 97672      | PASS                |
| 177            | 176             | 5               | 9               | 6.1          | 5932       | PASS                |