


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU011219\
Data File : VU029142.D
Acq On : 11 Jan 2019 15:18
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
Title : SW846 8260
Last Update : Sat Jan 12 01:33:59 2019

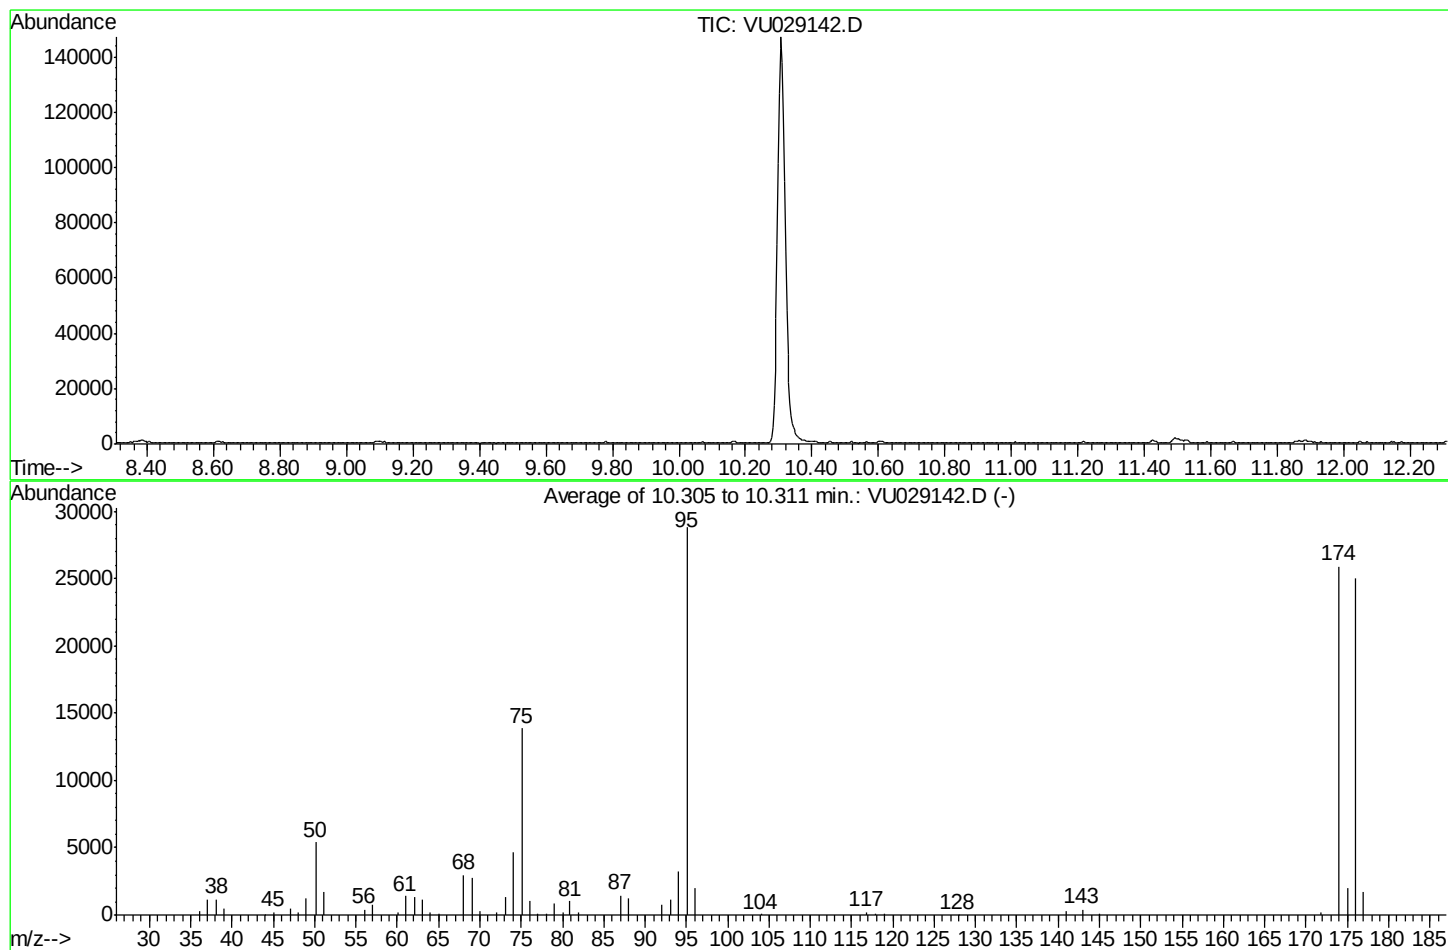

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	5399	PASS
75	95	30	60	48.2	13885	PASS
95	95	100	100	100.0	28821	PASS
96	95	5	9	6.9	1987	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	89.9	25912	PASS
175	174	5	9	7.7	2000	PASS
176	174	95	101	96.5	25013	PASS
177	176	5	9	7.0	1762	PASS