


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011221\
 Data File : VU041961.D
 Acq On : 12 Jan 2021 09:10
 Operator : SY/MD
 Sample : BFB62
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB602

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM011221WMA.M
 Title : VOC Analysis
 Last Update : Wed Jan 13 05:59:10 2021

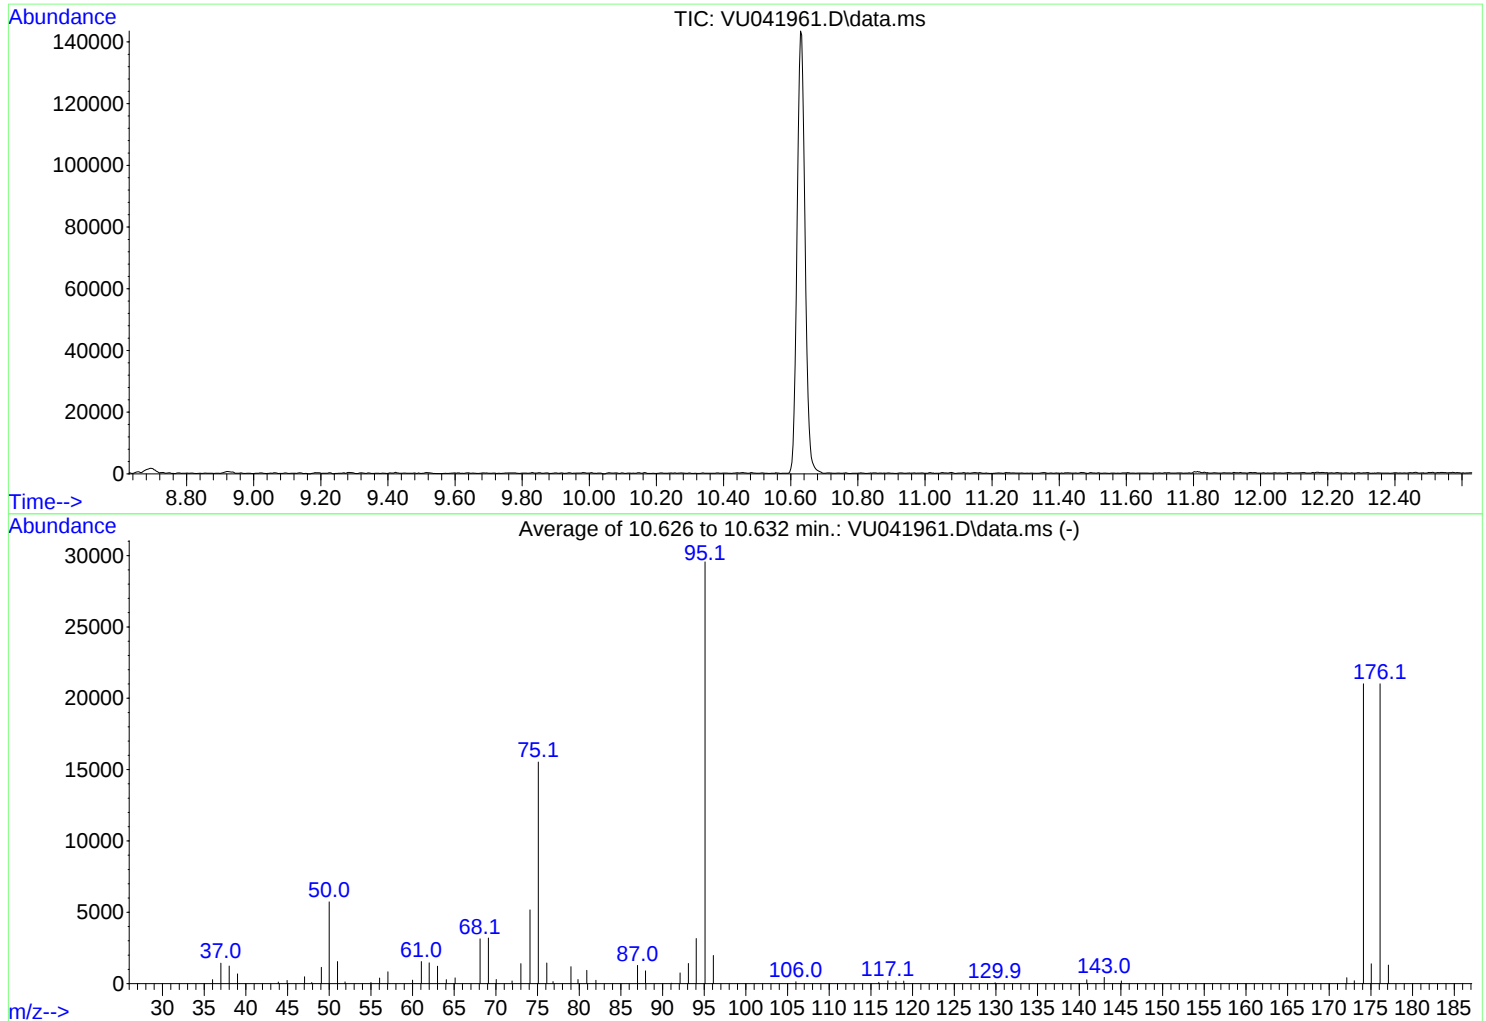

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	5733	PASS
75	95	30	80	52.5	15533	PASS
95	95	100	100	100.0	29560	PASS
96	95	5	9	6.7	1974	PASS
173	174	0.00	2	1.0	204	PASS
174	95	50	120	71.1	21011	PASS
175	174	5	9	6.6	1393	PASS
176	174	95	101	100.0	21011	PASS
177	176	5	9	6.2	1303	PASS

m/z	Abundance
44.00	224.0

Instrument :
MSVOA_U
ClientSampleId :
BFB602

m/z	Abundance
36.00	277.0
37.00	1298.0
38.00	1247.0
39.00	666.0
43.90	370.0
45.00	207.0
47.00	466.0
47.90	128.0
49.10	1224.0
50.00	5447.0
51.00	1683.0
51.90	131.0
55.00	112.0
56.00	384.0
57.00	825.0
60.00	260.0
61.00	1502.0
62.00	1389.0
63.00	1286.0
64.10	231.0
65.10	400.0
68.10	2984.0
69.10	3137.0
70.10	223.0
71.90	166.0
73.00	1292.0
74.10	4817.0
75.10	14727.0
76.10	1366.0
76.90	156.0
79.00	1132.0
79.90	279.0
80.90	928.0
82.00	229.0
87.00	1186.0
88.00	940.0
91.10	100.0
92.10	803.0
93.10	1400.0
94.00	2958.0
95.10	28072.0
96.10	1822.0
106.00	128.0
117.00	194.0
118.00	128.0
118.90	191.0
140.90	230.0
143.00	300.0
145.00	194.0
172.10	418.0
173.00	294.0
174.10	19416.0
175.00	1318.0
176.10	19256.0
177.10	1140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB602

m/z	Abundance
36.00	297.0
37.00	1473.0
38.00	1293.0
39.00	703.0
43.90	360.0
45.00	227.0
47.00	507.0
47.90	100.0
49.00	1160.0
50.00	5971.0
51.00	1525.0
51.90	129.0
55.00	134.0
56.10	395.0
57.00	849.0
60.00	244.0
61.10	1543.0
62.00	1484.0
63.00	1255.0
64.00	294.0
65.10	437.0
68.10	3220.0
69.10	3306.0
70.00	308.0
71.90	204.0
73.00	1386.0
74.10	5440.0
75.10	15927.0
76.10	1528.0
76.80	140.0
79.00	1236.0
79.90	292.0
80.90	939.0
82.00	244.0
87.00	1349.0
88.00	925.0
92.10	781.0
93.10	1494.0
94.00	3189.0
95.10	30504.0
96.10	2049.0
106.00	144.0
116.00	134.0
117.00	216.0
118.00	150.0
118.90	185.0
129.90	110.0
140.90	275.0
143.00	438.0
145.00	191.0
172.10	433.0
173.00	319.0
174.10	21608.0
175.10	1398.0
176.10	21720.0
177.10	1348.0

Instrument :
MSVOA_U
ClientSampleId :
BFB602

m/z	Abundance
36.00	273.0
37.00	1536.0
38.00	1169.0
39.00	689.0
43.90	291.0
44.90	251.0
47.10	457.0
49.00	1045.0
50.00	5782.0
51.00	1423.0
51.90	109.0
56.10	416.0
57.10	830.0
60.00	229.0
61.10	1596.0
62.00	1513.0
63.00	1118.0
64.00	311.0
65.10	375.0
68.10	3228.0
69.10	3148.0
70.00	332.0
72.00	204.0
73.00	1525.0
74.10	5254.0
75.10	15945.0
76.10	1449.0
76.90	147.0
79.00	1207.0
79.80	320.0
80.90	915.0
82.00	245.0
87.00	1294.0
87.90	825.0
92.10	661.0
93.10	1354.0
94.10	3334.0
95.10	30104.0
96.10	2051.0
106.00	142.0
115.90	138.0
117.10	212.0
118.00	116.0
119.00	158.0
129.90	108.0
140.90	313.0
143.00	572.0
145.10	172.0
172.10	398.0
174.10	22008.0
175.10	1464.0
176.10	22056.0
177.10	1421.0

Instrument :
MSVOA_U
ClientSampleId :
BFB602