


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011223\
Data File : VU052655.D
Acq On : 12 Jan 2023 09:18
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U011123W.M
Title : SW846 8260
Last Update : Fri Jan 13 01:24:13 2023

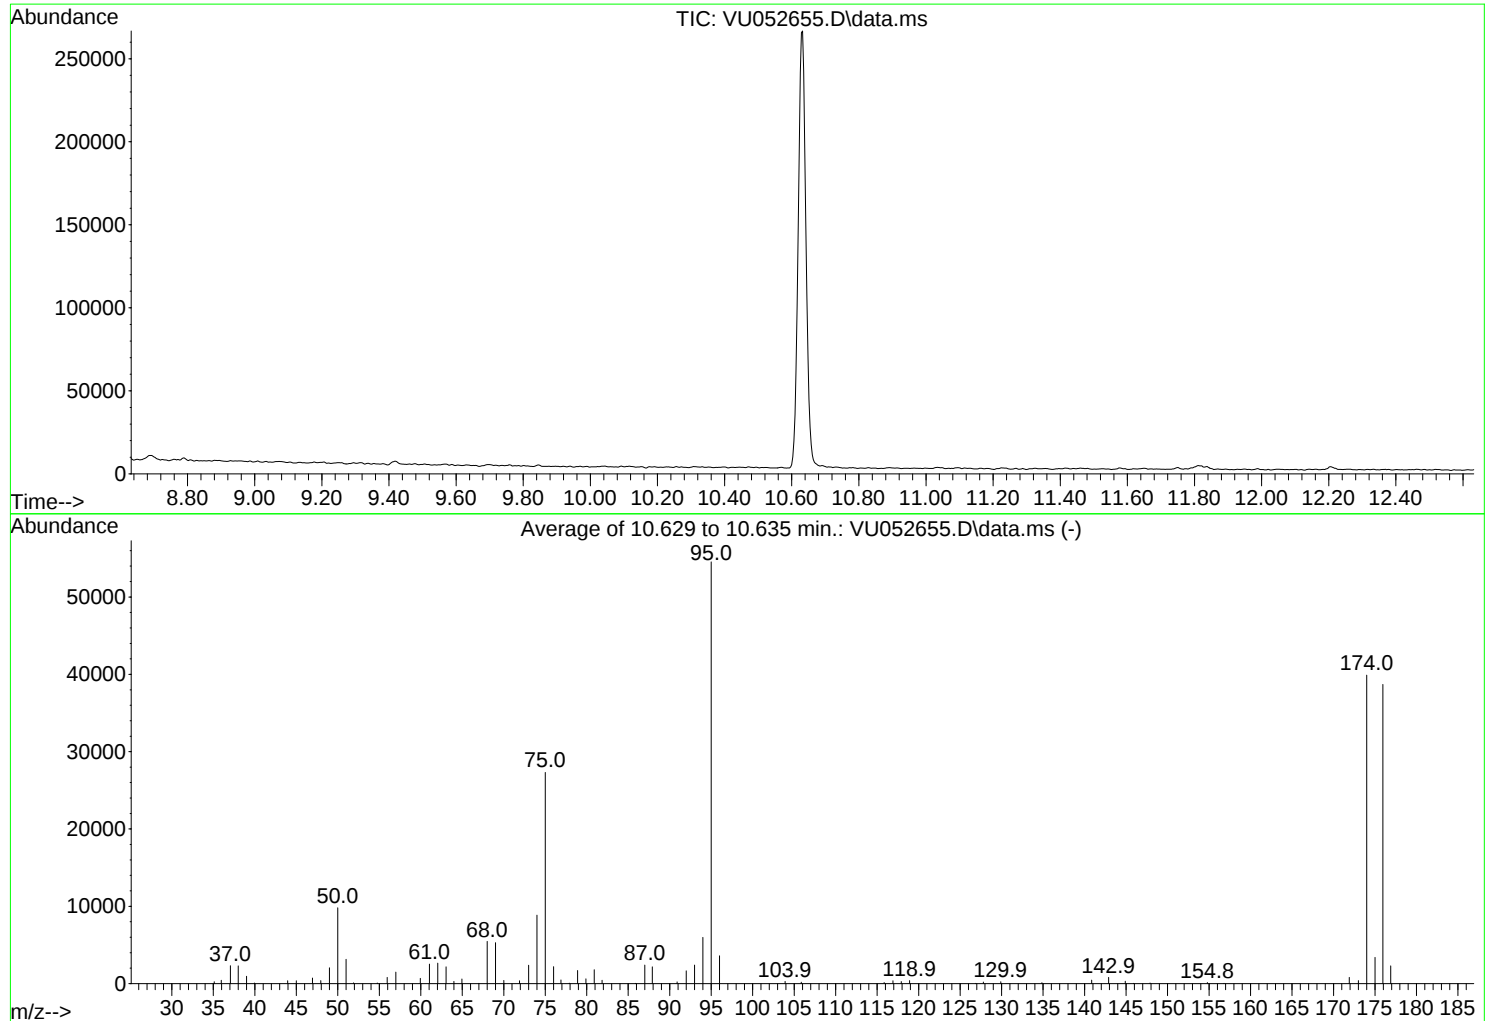

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	9810	PASS
75	95	30	60	50.1	27315	PASS
95	95	100	100	100.0	54547	PASS
96	95	5	9	6.6	3598	PASS
173	174	0.00	2	1.0	393	PASS
174	95	50	100	73.2	39904	PASS
175	174	5	9	8.5	3398	PASS
176	174	95	101	97.0	38691	PASS
177	176	5	9	5.9	2291	PASS