

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU011320\
 Data File : VU036441.D
 Acq On : 13 Jan 2020 17:23
 Operator : JC/MD
 Sample : L1090-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETOQ5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	79	85	95	rVB	167507	179491	10.63%	1.376%
2	1.932	177	184	197	rVB	163117	209114	12.39%	1.603%
3	2.594	379	390	404	rBV	302407	494777	29.32%	3.794%
4	3.015	518	521	524	rBV4	1538	1264	0.07%	0.010%
5	3.131	555	557	562	rVB4	1115	700	0.04%	0.005%
6	3.295	606	608	609	rBV	682	258	0.02%	0.002%
7	3.462	658	660	661	rBV2	541	214	0.01%	0.002%
8	3.539	683	684	685	rBV2	377	126	0.01%	0.001%
9	3.600	701	703	705	rBV2	669	374	0.02%	0.003%
10	3.652	716	719	721	rBV2	805	519	0.03%	0.004%
11	3.796	762	764	767	rBV3	626	345	0.02%	0.003%
12	3.854	780	782	784	rVB	572	227	0.01%	0.002%
13	3.935	804	807	808	rBV	985	507	0.03%	0.004%
14	4.086	852	854	855	rBV	765	352	0.02%	0.003%
15	4.134	867	869	870	rBV	279	114	0.01%	0.001%
16	4.153	871	875	877	rVV3	813	592	0.04%	0.005%
17	4.182	882	884	886	rBV3	371	191	0.01%	0.001%
18	4.253	905	906	908	rBV2	488	178	0.01%	0.001%
19	4.308	921	923	925	rBV	201	113	0.01%	0.001%
20	4.677	1023	1038	1062	rBV	168020	419552	24.86%	3.217%
21	5.108	1157	1172	1194	rBV	304562	677829	40.16%	5.197%
22	5.494	1290	1292	1294	rBV2	824	383	0.02%	0.003%
23	5.549	1306	1309	1313	rBV3	938	757	0.04%	0.006%
24	5.574	1313	1317	1318	rBV	668	496	0.03%	0.004%
25	5.626	1331	1333	1336	rVB3	774	282	0.02%	0.002%
26	5.767	1352	1377	1409	rBV2	620360	1687788	100.00%	12.941%
27	6.288	1523	1539	1562	rBV	567477	1092017	64.70%	8.373%
28	6.729	1661	1676	1699	rBV	394135	780312	46.23%	5.983%
29	7.127	1795	1800	1803	rBV5	1012	906	0.05%	0.007%
30	7.144	1803	1805	1811	rVV4	700	652	0.04%	0.005%
31	7.176	1813	1815	1817	rBV3	895	554	0.03%	0.004%
32	7.208	1817	1825	1837	rVV9	6921	15040	0.89%	0.115%
33	7.285	1847	1849	1850	rBV	421	146	0.01%	0.001%
34	7.311	1855	1857	1859	rBV3	564	308	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU011320\
 Data File : VU036441.D
 Acq On : 13 Jan 2020 17:23
 Operator : JC/MD
 Sample : L1090-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETOQ5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
 Title : VOC Analysis

35	7.385	1876	1880	1882	rBV2	883	656	0.04%	0.005%
36	7.520	1921	1922	1924	rBV2	353	134	0.01%	0.001%
37	7.600	1933	1947	1968	rBV	231458	423617	25.10%	3.248%
38	7.883	2031	2035	2036	rBV4	1034	681	0.04%	0.005%
39	7.931	2036	2050	2067	rBV	773140	1361266	80.65%	10.437%
40	8.211	2125	2137	2157	rBV2	159858	291897	17.29%	2.238%
41	8.459	2211	2214	2216	rBV	896	578	0.03%	0.004%
42	8.497	2220	2226	2235	rVV4	6376	10679	0.63%	0.082%
43	8.587	2248	2254	2258	rBV7	2215	2369	0.14%	0.018%
44	8.671	2268	2280	2326	rBV	355893	922044	54.63%	7.070%
45	8.925	2356	2359	2362	rBV2	1223	790	0.05%	0.006%
46	8.979	2374	2376	2380	rBV2	524	303	0.02%	0.002%
47	9.031	2391	2392	2398	rVB2	700	612	0.04%	0.005%
48	9.131	2419	2423	2427	rVB4	1043	921	0.05%	0.007%
49	9.182	2436	2439	2441	rBV	806	508	0.03%	0.004%
50	9.295	2471	2474	2477	rBV2	800	540	0.03%	0.004%
51	9.375	2493	2499	2506	rVB4	5963	8753	0.52%	0.067%
52	9.446	2509	2521	2558	rVB	776299	1379696	81.75%	10.579%
53	10.031	2700	2703	2705	rBV4	635	499	0.03%	0.004%
54	10.407	2818	2820	2826	rVB5	798	557	0.03%	0.004%
55	10.497	2843	2848	2850	rBV3	1979	1746	0.10%	0.013%
56	10.725	2915	2919	2922	rVB2	815	704	0.04%	0.005%
57	10.783	2923	2937	2957	rBV	540372	912657	54.07%	6.998%
58	10.880	2965	2967	2970	rBV	1256	854	0.05%	0.007%
59	11.095	3032	3034	3036	rBV2	734	359	0.02%	0.003%
60	11.571	3180	3182	3183	rBV	791	335	0.02%	0.003%
61	11.668	3210	3212	3214	rBV2	841	473	0.03%	0.004%
62	11.758	3238	3240	3241	rBV	2113	826	0.05%	0.006%
63	11.838	3252	3265	3288	rVB	612155	1080002	63.99%	8.281%
64	12.217	3371	3383	3400	rVB	620249	1056965	62.62%	8.104%
65	12.629	3508	3511	3512	rBV2	826	512	0.03%	0.004%
66	12.857	3580	3582	3585	rBV3	950	644	0.04%	0.005%
67	13.860	3887	3894	3901	rBV8	8556	12519	0.74%	0.096%


Sum of corrected areas: 13042174

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU011320\
Data File : VU036441.D
Acq On : 13 Jan 2020 17:23
Operator : JC/MD
Sample : L1090-09
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETOQ5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

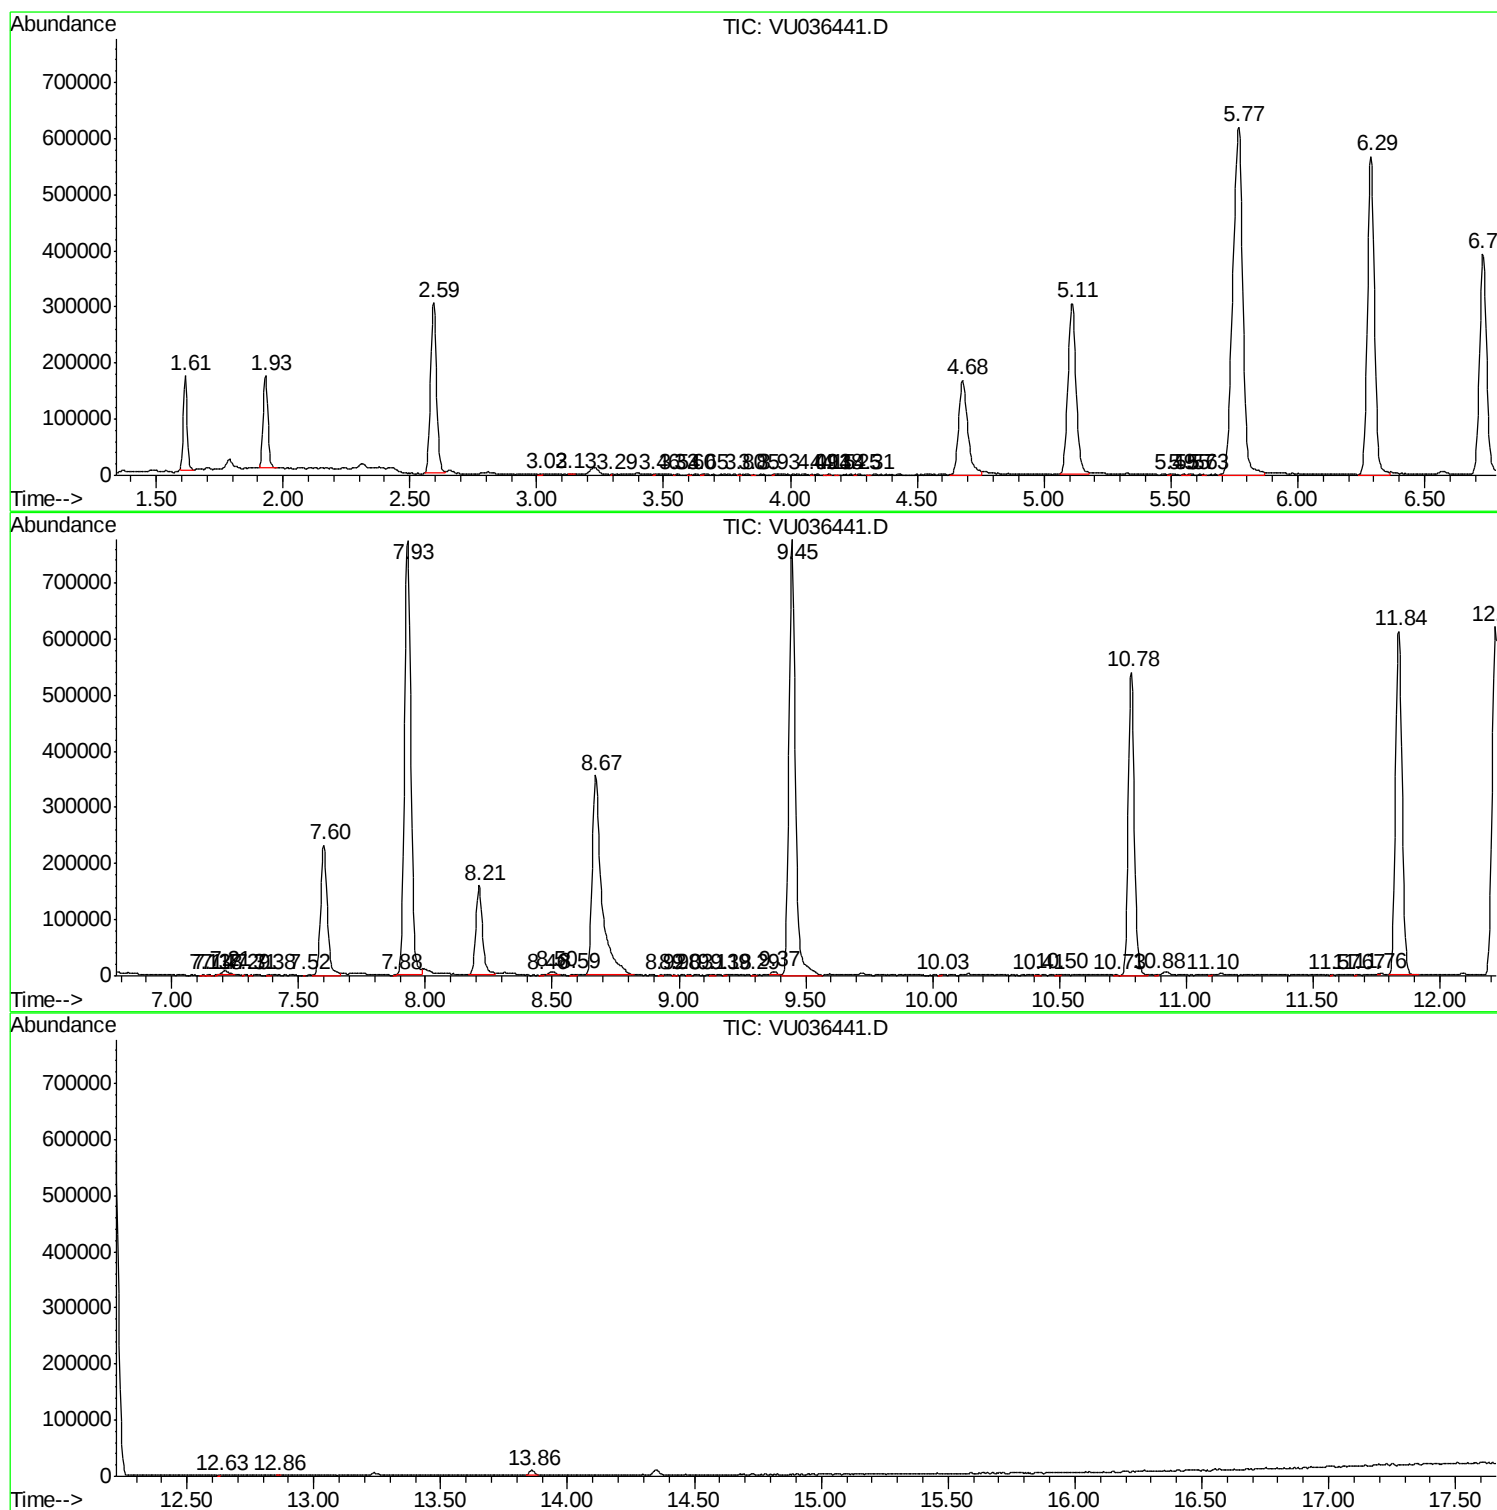

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU011320\
Data File : VU036441.D
Acq On : 13 Jan 2020 17:23
Operator : JC/MD
Sample : L1090-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETOQ5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU011320\
Data File : VU036441.D
Acq On : 13 Jan 2020 17:23
Operator : JC/MD
Sample : L1090-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETOQ5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc