


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU011320\
 Data File : VU036435.D
 Acq On : 13 Jan 2020 09:06
 Operator : JC/MD
 Sample : BFB38
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB38

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
 Title : VOC Analysis
 Last Update : Tue Jan 14 16:20:30 2020

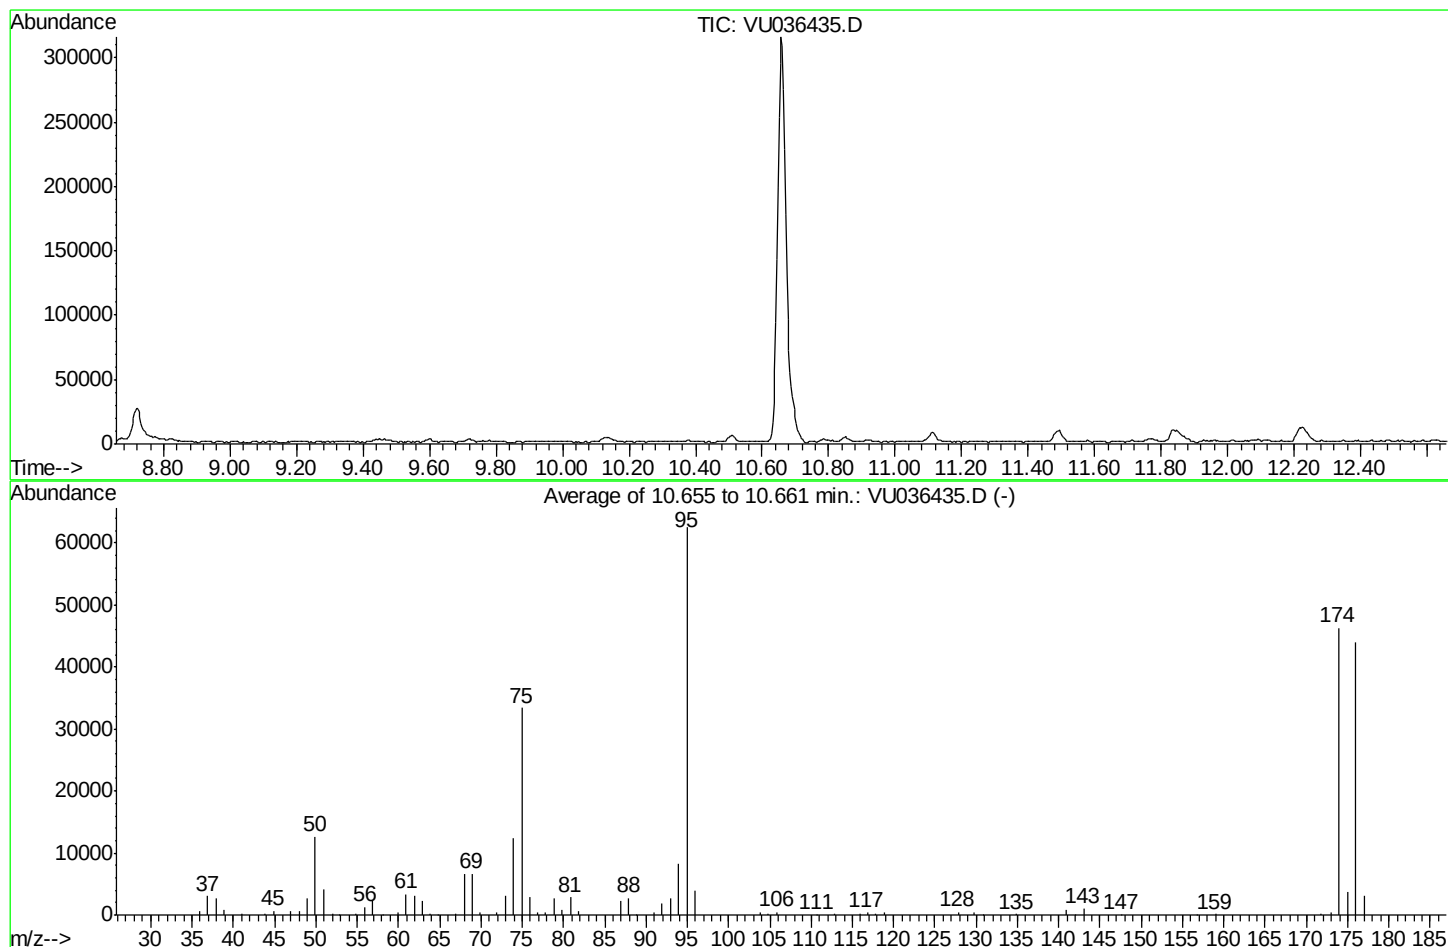

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	12690	PASS
75	95	30	80	53.5	33434	PASS
95	95	100	100	100.0	62522	PASS
96	95	5	9	6.2	3876	PASS
173	174	0.00	2	1.1	501	PASS
174	95	50	120	74.1	46314	PASS
175	174	5	9	7.8	3627	PASS
176	174	95	101	95.0	44010	PASS
177	176	5	9	6.9	3049	PASS

m/z	Abundance
35.90	613.0
36.90	2977.0
37.90	2981.0
38.80	1145.0
39.90	297.0
41.00	218.0
43.90	1047.0
44.80	711.0
46.90	798.0
47.90	504.0
48.90	2689.0
49.90	12562.0
50.90	3993.0
52.00	228.0
54.90	401.0
56.00	1382.0
56.90	2432.0
60.00	436.0
60.90	3285.0
61.90	2981.0
62.90	2113.0
63.80	263.0
66.90	247.0
67.90	6523.0
68.90	6507.0
69.90	415.0
71.80	524.0
73.00	2910.0
74.00	12446.0
75.00	33008.0
75.90	2657.0
76.90	597.0
77.90	426.0
78.80	2744.0
79.80	714.0
80.90	2831.0
81.80	492.0
86.90	2180.0
87.90	2710.0
90.90	457.0
92.00	1753.0
92.90	2600.0
93.90	7843.0
95.00	60472.0
96.00	3874.0
103.90	312.0
104.70	156.0
105.90	460.0
110.70	129.0
112.90	127.0
115.90	215.0
116.80	424.0
117.90	209.0
118.80	346.0
127.80	385.0
129.70	384.0
134.90	134.0
140.80	786.0
143.00	914.0
159.00	108.0
171.80	182.0
173.00	423.0
173.90	43384.0
175.00	3384.0
175.90	41168.0
176.90	2962.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
35.90	678.0
36.90	3159.0
38.00	2825.0
38.90	1129.0
39.90	307.0
41.00	198.0
43.90	1101.0
44.80	658.0
46.90	658.0
47.90	565.0
48.90	2771.0
49.90	12990.0
50.90	4300.0
52.00	211.0
54.90	376.0
55.90	1317.0
56.90	2383.0
58.10	158.0
60.00	521.0
60.90	3446.0
62.00	3169.0
62.90	2296.0
63.80	279.0
66.90	286.0
68.00	6931.0
69.00	6717.0
69.90	413.0
71.90	514.0
73.00	3197.0
74.00	12773.0
75.00	34696.0
75.90	2893.0
76.90	543.0
77.80	443.0
78.80	2835.0
79.90	827.0
80.80	2860.0
81.90	583.0
86.90	2286.0
87.90	2829.0
88.70	151.0
91.00	372.0
92.00	1960.0
92.90	2785.0
93.90	8629.0
95.00	64552.0
96.00	4008.0
103.90	375.0
104.80	192.0
105.90	459.0
110.70	103.0
112.90	193.0
115.90	234.0
116.80	383.0
117.80	253.0
118.80	408.0
127.80	482.0
129.70	335.0
134.90	149.0
140.80	916.0
142.00	131.0
143.00	1005.0
159.00	138.0
171.80	163.0
173.00	481.0
173.90	47920.0
174.90	3827.0
175.90	45208.0
176.90	3198.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

m/z	Abundance
35.80	642.0
36.90	3111.0
37.90	2406.0
38.90	1031.0
40.00	309.0
41.10	195.0
43.90	1162.0
44.90	581.0
46.90	591.0
48.00	600.0
48.90	2573.0
49.90	12519.0
50.90	4134.0
52.00	191.0
52.90	101.0
54.90	319.0
55.90	1259.0
56.90	2010.0
58.10	149.0
60.00	600.0
60.90	3419.0
62.00	3120.0
62.90	2370.0
63.80	272.0
64.70	107.0
66.90	330.0
68.00	6696.0
69.00	6771.0
69.90	387.0
72.00	454.0
73.00	3091.0
73.90	11915.0
75.00	32600.0
75.90	3044.0
76.90	402.0
77.80	370.0
78.80	2734.0
79.90	945.0
80.80	2909.0
81.90	667.0
86.90	2237.0
87.90	2609.0
88.80	159.0
91.10	313.0
91.90	2085.0
93.00	2984.0
93.90	8358.0
95.00	62544.0
96.00	3748.0
103.90	335.0
104.80	170.0
105.90	391.0
112.90	204.0
116.00	232.0
116.80	378.0
117.80	309.0
118.80	433.0
127.80	433.0
129.80	256.0
130.80	110.0
134.90	178.0
140.90	971.0
141.90	104.0
143.00	1031.0
147.60	145.0
156.70	106.0
159.00	186.0
171.80	129.0
173.00	599.0
173.90	47640.0
174.90	3670.0
175.90	45656.0
177.00	2988.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38

Scan 2884 (10.613 min): VU036435.D
BFB38

m/z	Abundance
39.00	264.0
39.90	321.0
40.80	101.0
43.10	162.0
43.80	926.0
54.80	194.0
68.00	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB38