

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011321\
 Data File : VU041986.D
 Acq On : 13 Jan 2021 17:28
 Operator : SY/MD
 Sample : M1026-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXM1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC: VU041986.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.491	38	47	52	rBV5	4851	6628	1.09%	0.147%
2	1.604	74	82	94	rVB	63473	68613	11.27%	1.518%
3	1.919	171	180	193	rBV	62255	79587	13.08%	1.761%
4	2.578	373	385	399	rBV	108145	177596	29.18%	3.930%
5	3.057	521	534	546	rVB2	4464	7660	1.26%	0.170%
6	4.652	1013	1030	1080	rBV2	87119	288142	47.34%	6.377%
7	5.079	1146	1163	1188	rBV2	95402	215665	35.43%	4.773%
8	5.738	1347	1368	1386	rBV3	180437	472372	77.61%	10.454%
9	6.259	1514	1530	1548	rBV	142152	268699	44.15%	5.947%
10	6.552	1607	1621	1640	rBV	149908	282139	46.36%	6.244%
11	6.703	1653	1668	1684	rBV2	108015	207412	34.08%	4.590%
12	7.574	1924	1939	1960	rBV	54877	96312	15.82%	2.131%
13	7.906	2028	2042	2057	rBV	202921	351709	57.79%	7.784%
14	8.185	2115	2129	2145	rBV2	35504	61629	10.13%	1.364%
15	8.555	2230	2244	2258	rBV	149846	251213	41.28%	5.560%
16	8.639	2258	2270	2303	rVV	324912	608631	100.00%	13.470%
17	9.420	2498	2513	2546	rVB	216871	367435	60.37%	8.132%
18	10.754	2916	2928	2943	rVB	85499	137507	22.59%	3.043%
19	11.809	3244	3256	3272	rBV	176295	284491	46.74%	6.296%
20	12.188	3362	3374	3390	rVB	177535	285100	46.84%	6.310%




Sum of corrected areas: 4518540

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011321\
Data File : VU041986.D
Acq On : 13 Jan 2021 17:28
Operator : SY/MD
Sample : M1026-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXM1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

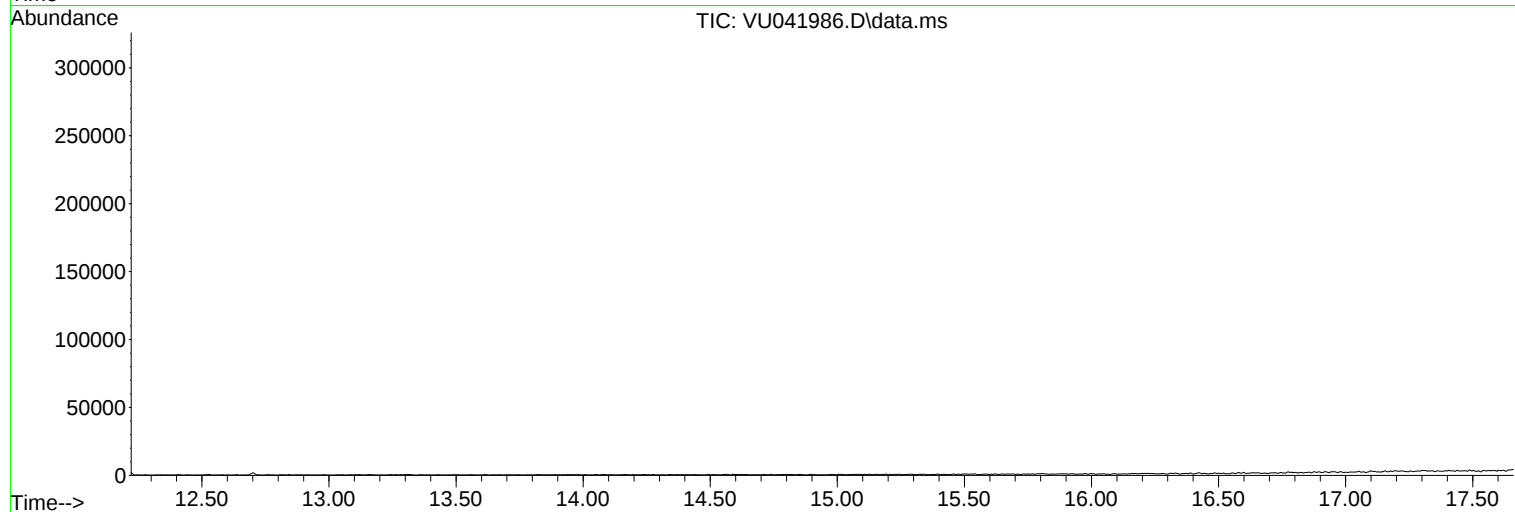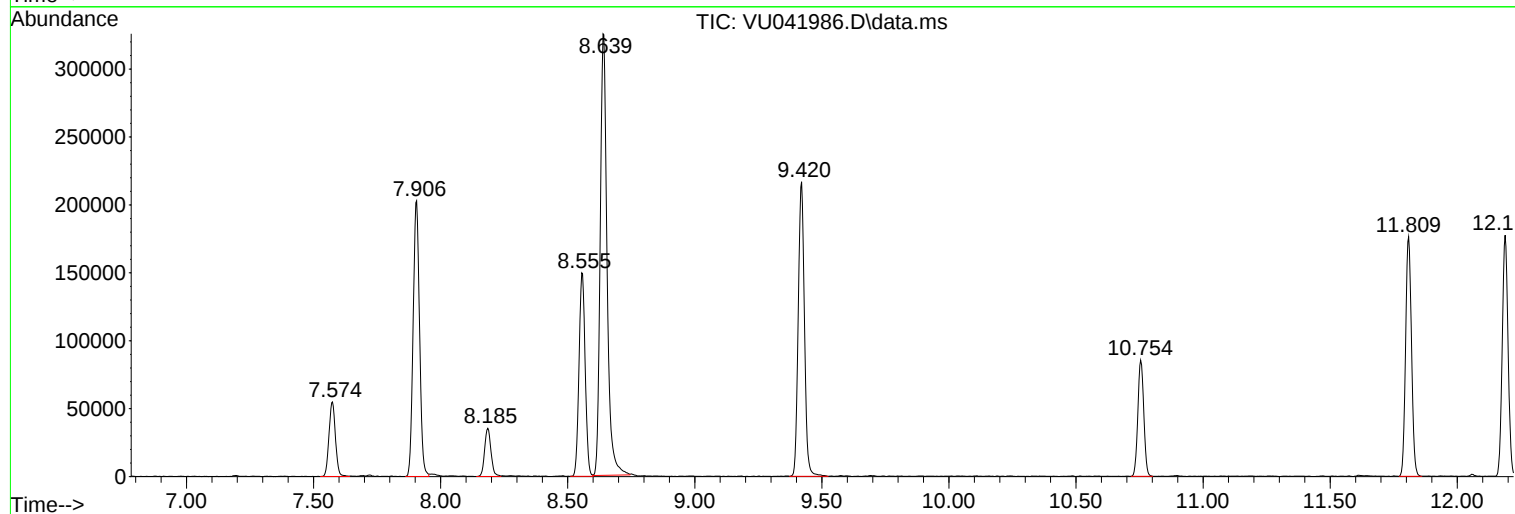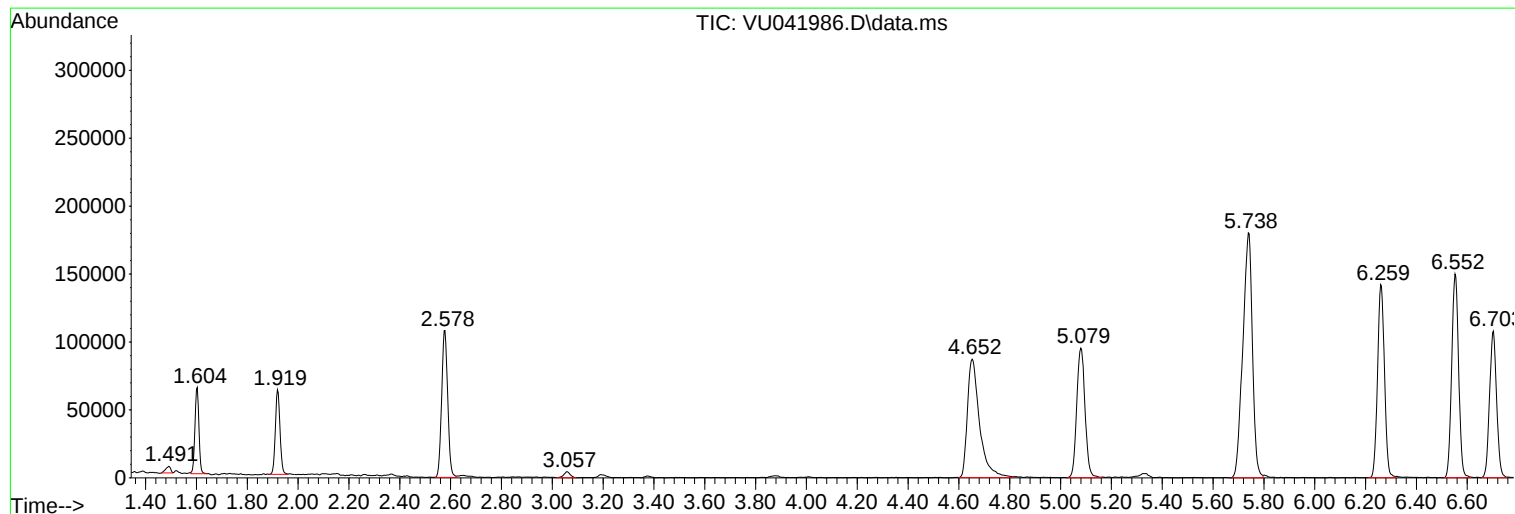

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011321\
Data File : VU041986.D
Acq On : 13 Jan 2021 17:28
Operator : SY/MD
Sample : M1026-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXM1










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.574	1.79 ug/L	96312	1,4-Difluorobenzene	6.259

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	37
2			Thiophosgene	114	CCl2S	000463-71-8	28
3			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	25
4			1,3-Cyclohexadiene	80	C6H8	000592-57-4	25
5			2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	23

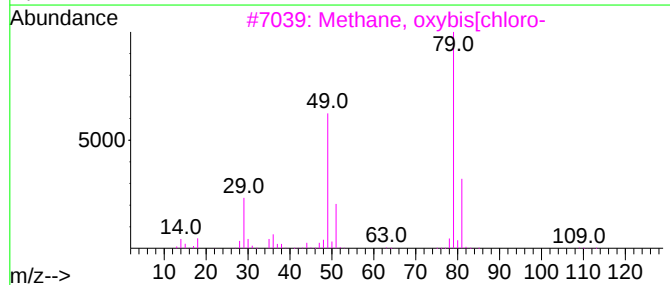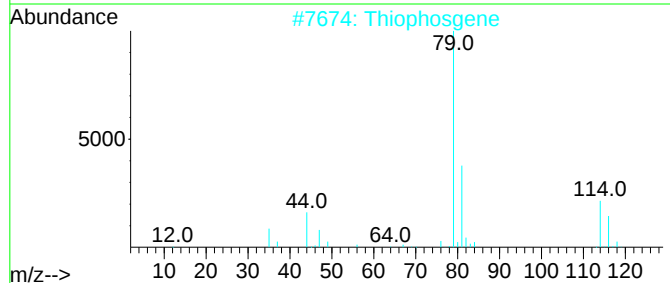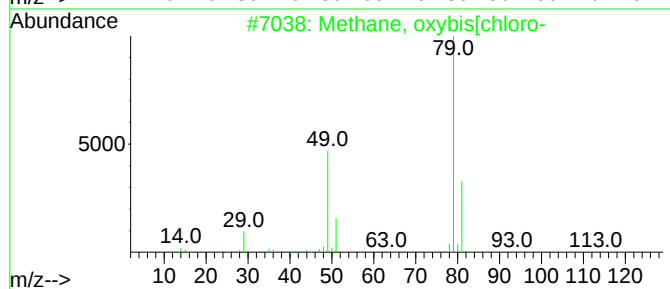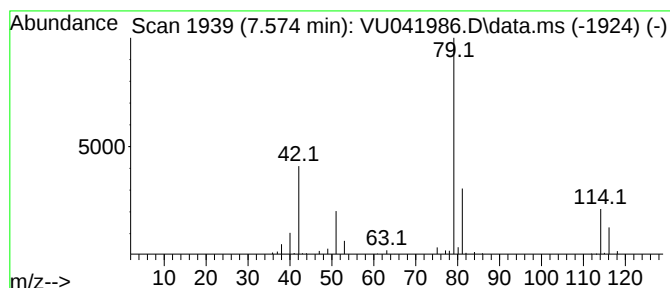

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011321\
Data File : VU041986.D
Acq On : 13 Jan 2021 17:28
Operator : SY/MD
Sample : M1026-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXM1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.574	1.8	ug/L	96312	1	6.259	268699	5.0