

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011321\
 Data File : VU041990.D
 Acq On : 13 Jan 2021 19:05
 Operator : SY/MD
 Sample : M1027-01DL 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXM2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC: VU041990.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	91	rVB	63684	66620	11.81%	1.666%
2	1.919	172	180	189	rBV	61222	73818	13.08%	1.845%
3	2.144	237	250	261	rVB	111822	161984	28.71%	4.050%
4	2.575	372	384	404	rBV	105735	172039	30.49%	4.301%
5	3.057	524	534	547	rVB2	8958	16238	2.88%	0.406%
6	4.665	1016	1034	1086	rBV	62084	276000	48.92%	6.900%
7	5.080	1146	1163	1184	rBV2	91643	201148	35.65%	5.029%
8	5.739	1347	1368	1388	rBV3	198934	511851	90.72%	12.796%
9	6.260	1518	1530	1544	rBV	138930	257915	45.71%	6.448%
10	6.552	1611	1621	1630	rBV9	7672	13855	2.46%	0.346%
11	6.700	1651	1667	1688	rBV	104766	204908	36.32%	5.123%
12	7.575	1926	1939	1956	rBV	50245	88745	15.73%	2.219%
13	7.903	2029	2041	2059	rBV	189613	326375	57.85%	8.159%
14	8.186	2118	2129	2147	rBV	34470	59666	10.58%	1.492%
15	8.642	2258	2271	2302	rBV	293335	564214	100.00%	14.106%
16	9.420	2498	2513	2531	rBV	190046	321323	56.95%	8.033%
17	10.755	2917	2928	2940	rBV	85537	138311	24.51%	3.458%
18	11.809	3244	3256	3273	rVB	174629	273841	48.53%	6.846%
19	12.189	3361	3374	3388	rBV	169390	271095	48.05%	6.777%




Sum of corrected areas: 3999946

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011321\
Data File : VU041990.D
Acq On : 13 Jan 2021 19:05
Operator : SY/MD
Sample : M1027-01DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXM2DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

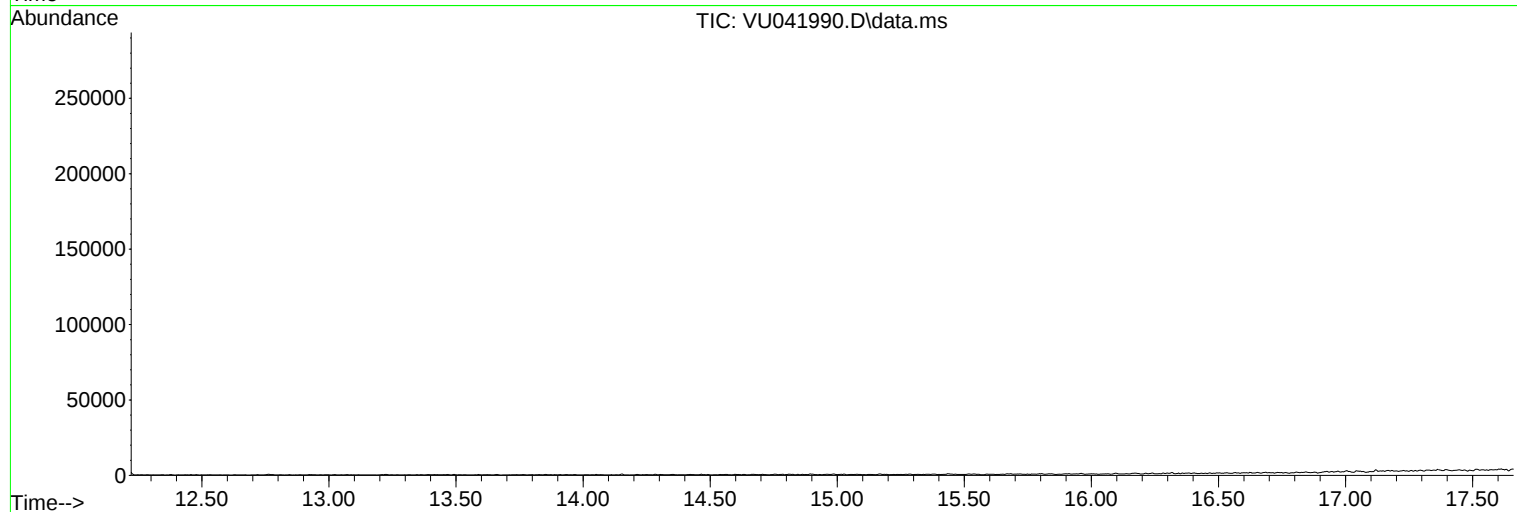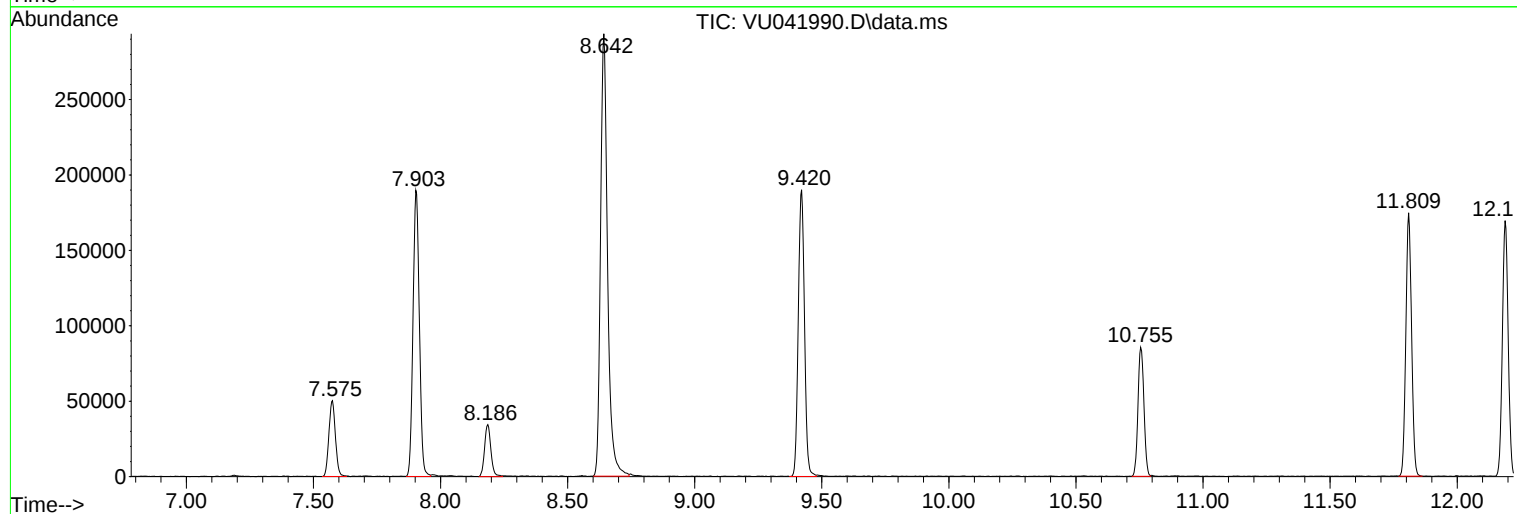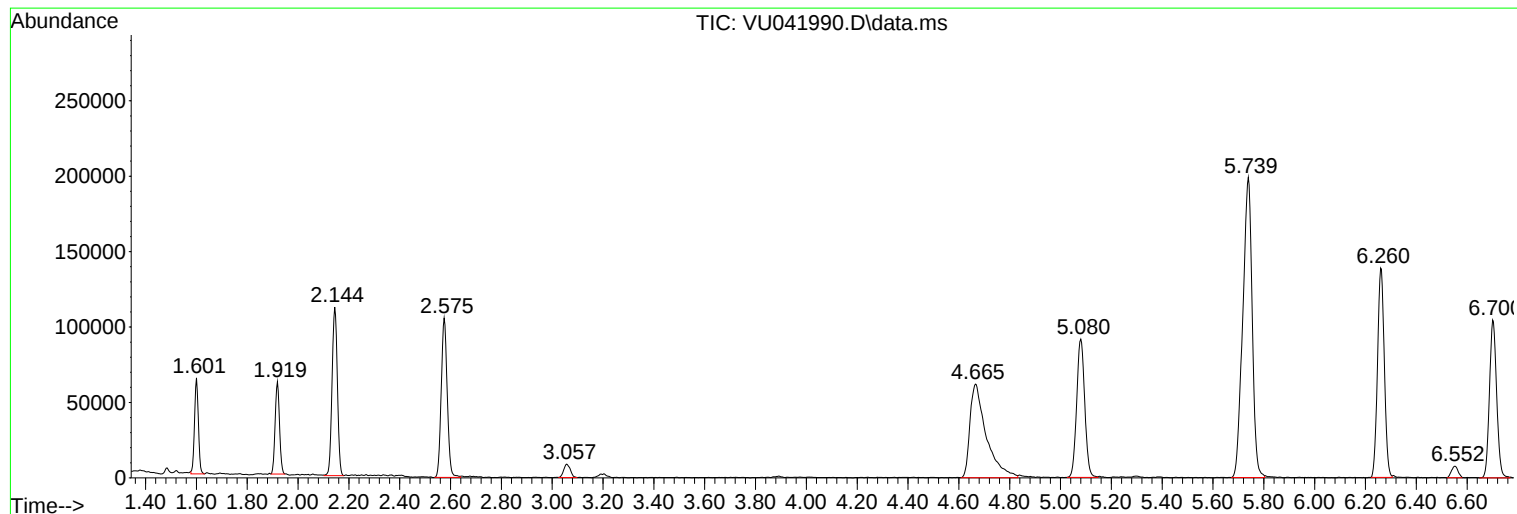

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011321\
Data File : VU041990.D
Acq On : 13 Jan 2021 19:05
Operator : SY/MD
Sample : M1027-01DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXM2DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011321\
Data File : VU041990.D
Acq On : 13 Jan 2021 19:05
Operator : SY/MD
Sample : M1027-01DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXM2DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
