


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011321\
Data File : VU041973.D
Acq On : 13 Jan 2021 10:01
Operator : SY/MD
Sample : BFB35
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB35

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat Jan 16 01:05:16 2021

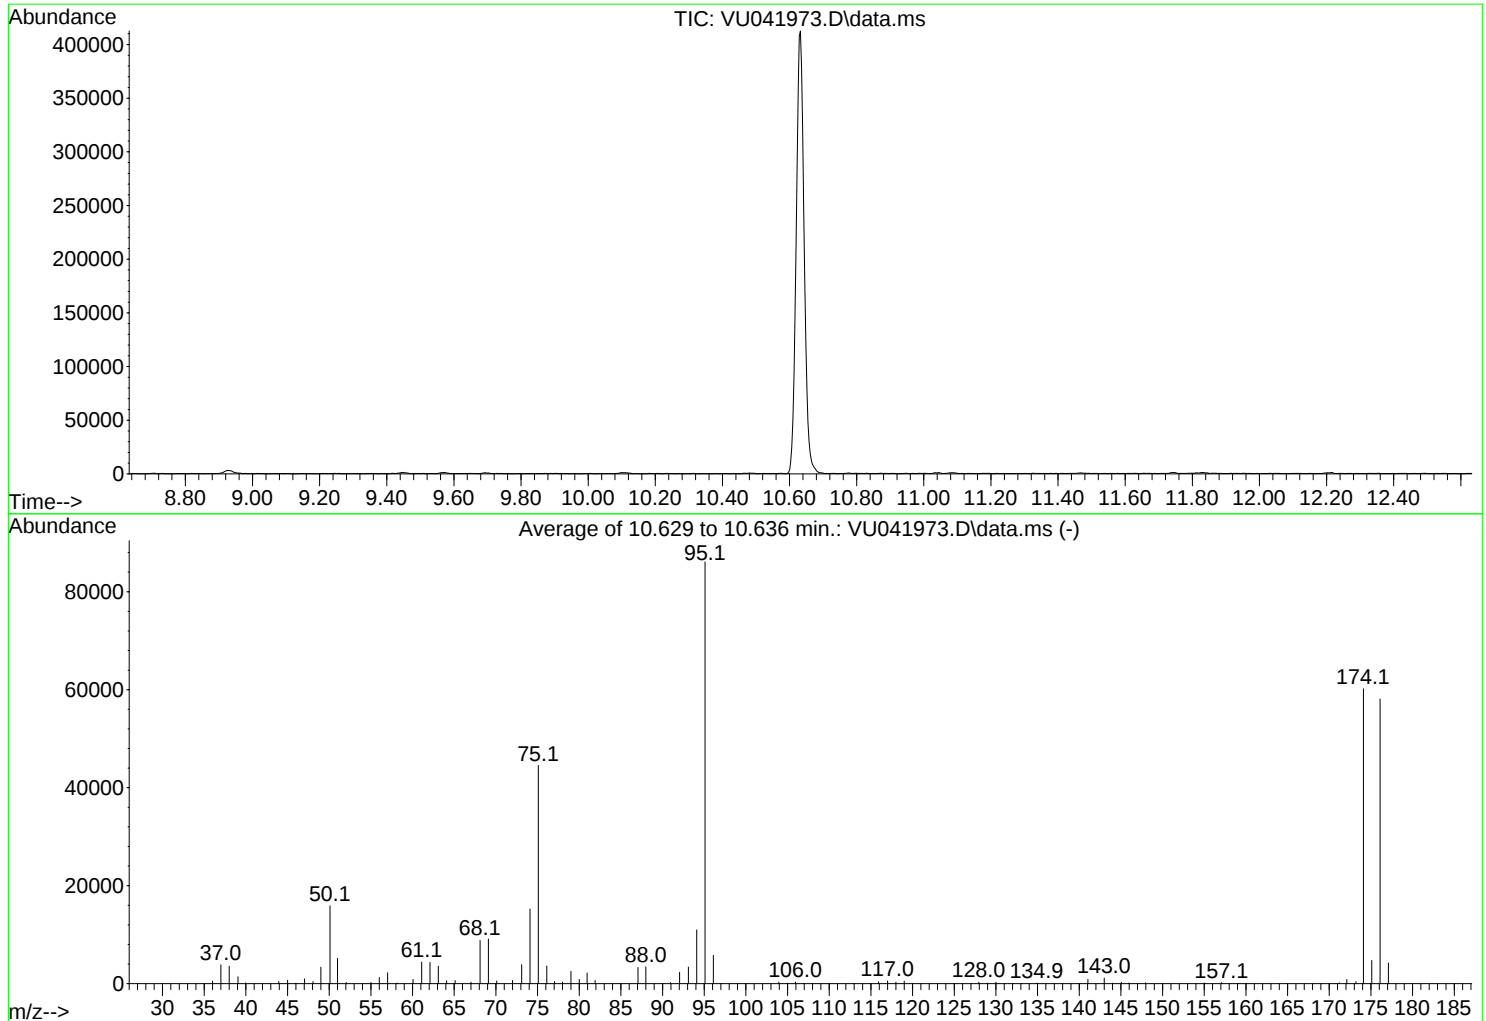

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	15861	PASS
75	95	30	80	51.7	44547	PASS
95	95	100	100	100.0	86104	PASS
96	95	5	9	6.7	5799	PASS
173	174	0.00	2	0.7	416	PASS
174	95	50	120	69.9	60192	PASS
175	174	5	9	7.9	4753	PASS
176	174	95	101	96.5	58115	PASS
177	176	5	9	7.2	4212	PASS

m/z	Abundance
43.90	249.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35

m/z	Abundance
36.00	525.0
37.00	4142.0
38.00	3571.0
39.10	1436.0
40.00	182.0
44.00	671.0
45.00	722.0
46.00	170.0
47.10	940.0
48.00	426.0
49.00	3634.0
50.10	16528.0
51.00	5363.0
52.00	252.0
55.00	202.0
56.00	1333.0
57.00	2350.0
58.10	129.0
60.10	1062.0
61.10	4504.0
62.10	4279.0
63.10	3634.0
64.10	655.0
65.10	736.0
67.00	284.0
68.10	9197.0
69.10	9243.0
70.10	596.0
72.00	724.0
73.10	4014.0
74.10	15595.0
75.10	46096.0
76.10	3725.0
77.00	447.0
77.90	314.0
79.00	2695.0
80.00	827.0
80.90	2305.0
81.90	684.0
87.10	3439.0
88.00	3170.0
91.00	291.0
92.00	2282.0
93.10	3427.0
94.10	11445.0
95.10	88080.0
96.10	5944.0
103.90	309.0
105.00	151.0
106.00	304.0
106.90	112.0
115.90	343.0
117.00	557.0
118.00	276.0
119.00	487.0
128.00	335.0
129.00	157.0
130.00	265.0
141.10	884.0
143.00	1227.0
145.10	304.0
146.00	139.0
148.00	201.0
155.00	132.0
157.10	275.0
159.10	111.0
170.80	103.0
171.20	158.0
172.10	874.0
174.10	59872.0
175.10	4826.0
176.10	58672.0
177.10	4252.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35

m/z	Abundance
36.00	543.0
37.00	3954.0
38.00	3673.0
39.10	1484.0
39.90	177.0
44.00	655.0
45.00	695.0
46.00	117.0
47.00	1036.0
48.10	430.0
49.00	3468.0
50.10	16334.0
51.00	5362.0
52.10	239.0
55.00	250.0
56.00	1289.0
57.00	2315.0
58.20	165.0
60.00	910.0
61.10	4638.0
62.10	4462.0
63.10	3647.0
64.10	617.0
65.10	638.0
67.00	317.0
68.10	9108.0
69.10	9414.0
70.10	589.0
72.00	709.0
73.10	4065.0
74.10	15716.0
75.10	45840.0
76.10	3680.0
77.00	452.0
78.00	340.0
79.00	2585.0
80.00	871.0
81.00	2241.0
81.90	649.0
87.10	3379.0
88.00	3579.0
90.90	200.0
92.10	2384.0
93.10	3520.0
94.10	11361.0
95.10	88800.0
96.10	6032.0
97.00	102.0
103.90	321.0
105.00	125.0
106.00	344.0
106.90	102.0
112.90	101.0
115.90	420.0
117.00	544.0
118.00	307.0
119.00	531.0
128.00	351.0
129.00	145.0
130.00	293.0
131.00	114.0
134.90	130.0
141.10	902.0
143.00	1211.0
144.00	118.0
145.00	296.0
146.00	140.0
148.00	187.0
155.00	148.0
157.10	241.0
171.20	190.0
172.10	893.0
174.10	62144.0
175.10	4917.0
176.10	59864.0
177.10	4440.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35

m/z	Abundance
36.00	541.0
37.00	3464.0
38.00	3460.0
39.00	1292.0
39.90	163.0
44.00	657.0
45.00	634.0
47.00	1021.0
48.10	400.0
49.00	3033.0
50.10	14722.0
51.00	4783.0
52.10	170.0
55.00	256.0
56.00	1109.0
57.00	1962.0
58.20	130.0
60.00	720.0
61.10	4131.0
62.10	4286.0
63.10	3382.0
64.10	550.0
65.10	609.0
67.00	268.0
68.10	8173.0
69.10	8709.0
70.10	524.0
72.00	561.0
73.10	3614.0
74.10	14409.0
75.10	41704.0
76.10	3349.0
77.10	398.0
78.10	363.0
79.00	2264.0
80.00	823.0
81.00	2074.0
81.90	634.0
87.00	3103.0
88.00	3561.0
91.00	160.0
92.10	2338.0
93.10	3206.0
94.10	10080.0
95.10	81432.0
96.10	5420.0
104.00	345.0
105.90	369.0
115.90	360.0
117.00	588.0
118.00	333.0
119.00	522.0
127.90	297.0
130.00	314.0
131.10	125.0
134.90	143.0
141.00	822.0
143.00	1033.0
144.00	145.0
145.00	302.0
145.90	124.0
147.90	178.0
155.00	134.0
157.10	198.0
171.20	180.0
172.10	809.0
173.20	1247.0
174.10	58560.0
175.10	4516.0
176.10	55808.0
177.10	3944.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35