

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011323\
 Data File : VU052673.D
 Acq On : 13 Jan 2023 12:41
 Operator : JC/MD
 Sample : 01139-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH1Z7

Quant Time: Jan 13 22:25:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 11 00:53:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	149899	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	149477	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	65069	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	51674	3.924	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	78.400%	
7) Chloroethane-d5	1.916	69	45007	4.195	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	83.800%	
11) 1,1-Dichloroethene-d2	2.565	65	24294	4.189	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	83.800%	
20) 2-Butanone-d5	4.639	46	156950	44.573	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	89.140%	
24) Chloroform-d	5.060	84	111101	4.523	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.400%	
26) 1,2-Dichloroethane-d4	5.700	65	58430	4.632	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.600%	
32) Benzene-d6	5.723	84	220653	4.554	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.000%	
36) 1,2-Dichloropropane-d6	6.687	67	73319	4.541	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	90.800%	
41) Toluene-d8	7.896	98	178830	4.187	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	83.800%	
43) trans-1,3-Dichloroprop...	8.176	79	25295	4.213	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	84.200%	
46) 2-Hexanone-d5	8.632	63	105931	42.473	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	84.940%	
56) 1,1,2,2-Tetrachloroeth...	10.751	84	54037	4.372	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	87.400%	
66) 1,2-Dichlorobenzene-d4	12.189	152	64661	5.459	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	109.200%	
Target Compounds					Qvalue	
13) Acetone	2.671	43	13608	5.389	ug/L	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011323\
Data File : VU052673.D
Acq On : 13 Jan 2023 12:41
Operator : JC/MD
Sample : 01139-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH1Z7

Quant Time: Jan 13 22:25:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 11 00:53:59 2023
Response via : Initial Calibration

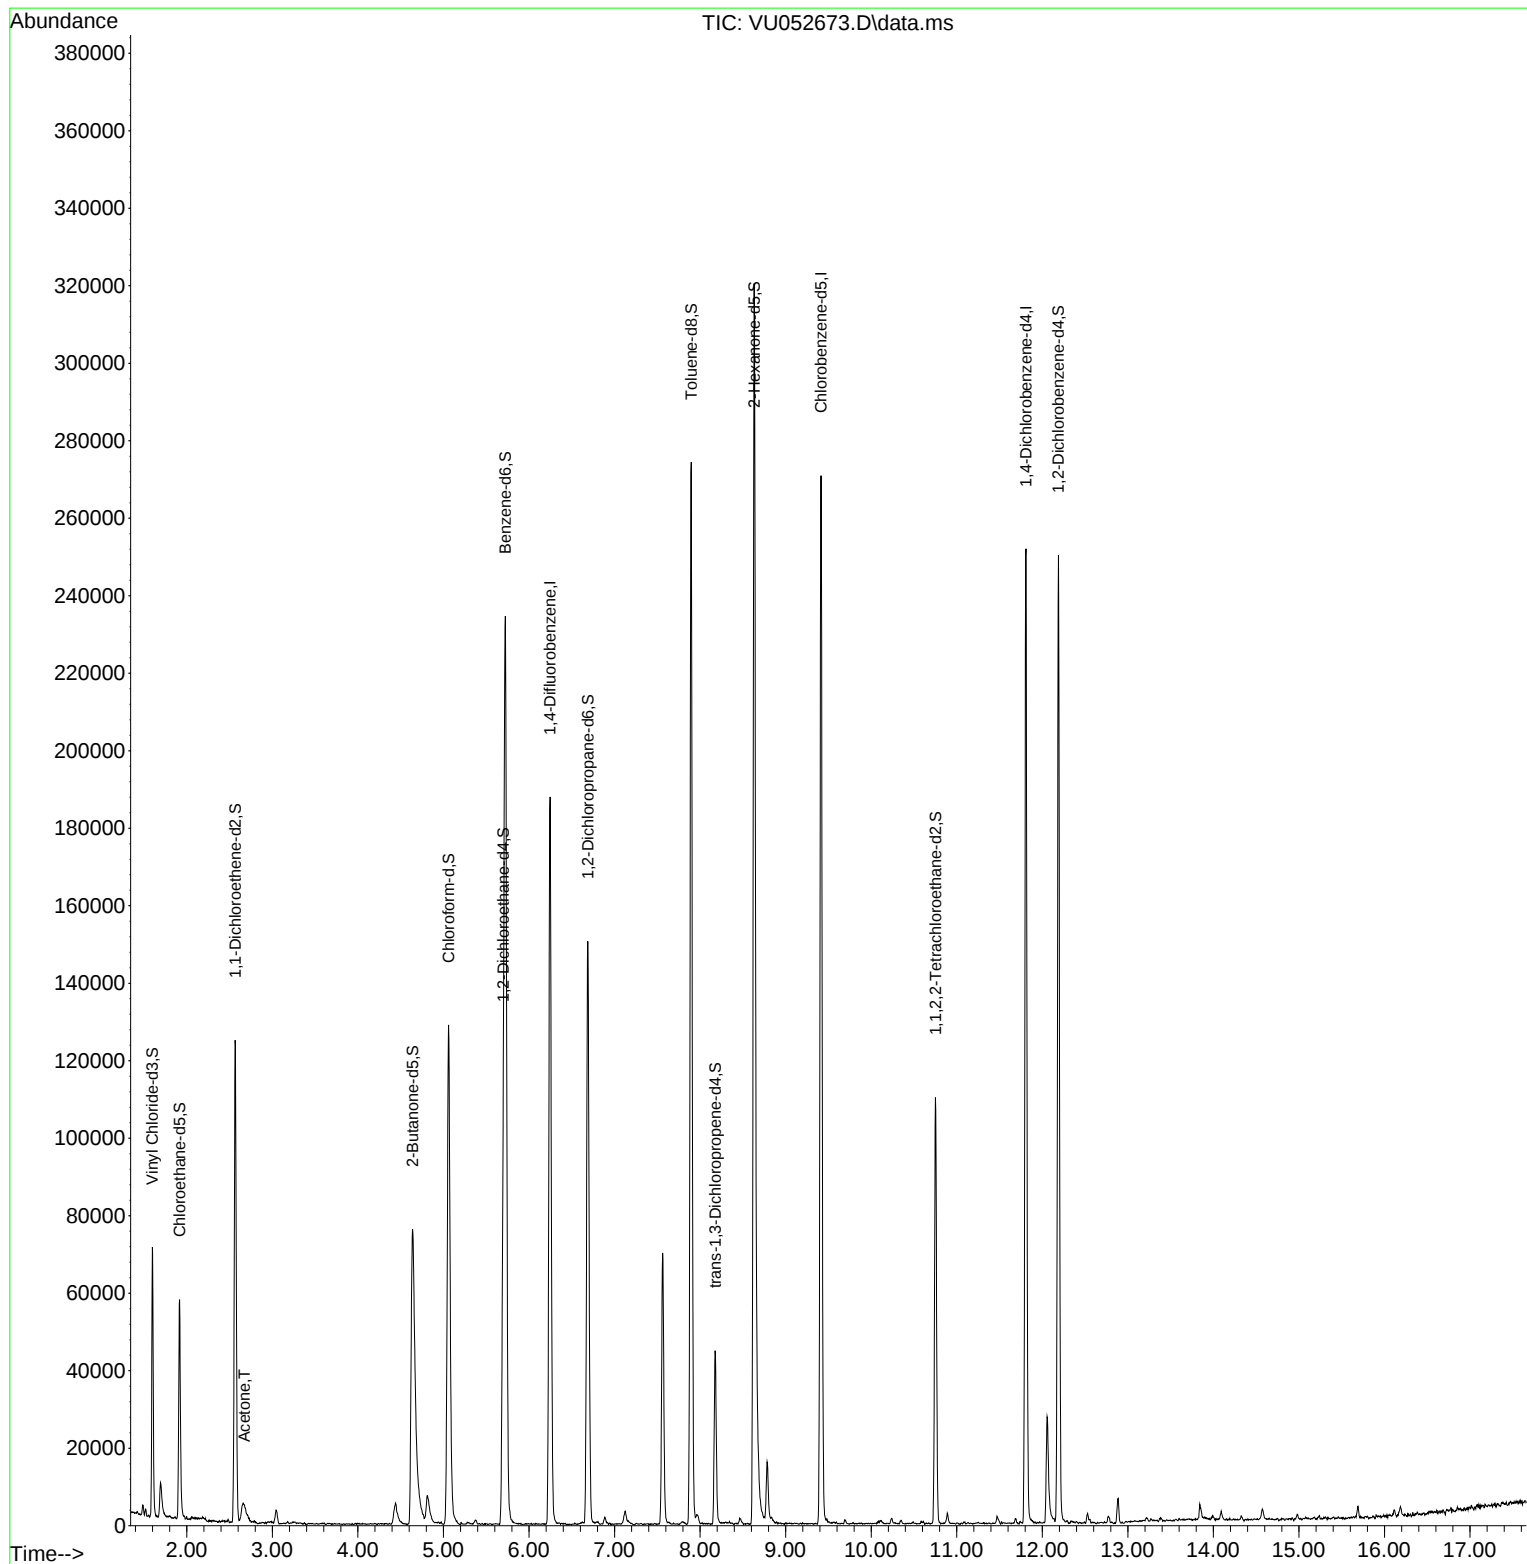

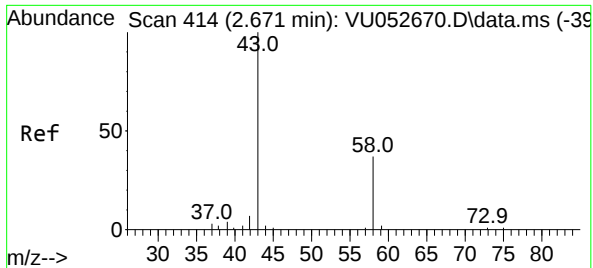

#13
 Acetone
 Concen: 5.389 ug/L
 RT: 2.671 min Scan# 41
 Delta R.T. 0.010 min
 Lab File: VU052673.D
 Acq: 13 Jan 2023 12:41

Instrument :
 MSVOA_U
 ClientSampleId :
 BH1Z7

Tgt Ion: 43 Resp: 13608
 Ion Ratio Lower Upper
 43 100
 58 19.9 0.0 68.8

