

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011323\
 Data File : VU052675.D
 Acq On : 13 Jan 2023 13:29
 Operator : JC/MD
 Sample : 01139-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH1Z9

Quant Time: Jan 13 22:26:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 11 00:53:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	141405	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	141086	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	64735	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	51595	4.153	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	83.000%	
7) Chloroethane-d5	1.916	69	45244	4.470	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	89.400%	
11) 1,1-Dichloroethene-d2	2.565	65	24310	4.444	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	88.800%	
20) 2-Butanone-d5	4.636	46	161546	48.634	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	97.260%	
24) Chloroform-d	5.060	84	111970	4.832	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.600%	
26) 1,2-Dichloroethane-d4	5.700	65	59854	5.030	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.600%	
32) Benzene-d6	5.726	84	224530	4.910	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.200%	
36) 1,2-Dichloropropane-d6	6.687	67	74089	4.862	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.200%	
41) Toluene-d8	7.896	98	180746	4.483	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	89.600%	
43) trans-1,3-Dichloroprop...	8.176	79	25614	4.520	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.400%	
46) 2-Hexanone-d5	8.632	63	108190	45.959	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	91.920%	
56) 1,1,2,2-Tetrachloroeth...	10.751	84	55046	4.718	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.400%	
66) 1,2-Dichlorobenzene-d4	12.188	152	64250	5.452	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	109.000%	
Target Compounds						
13) Acetone	2.661	43	11971	5.025	ug/L	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011323\
Data File : VU052675.D
Acq On : 13 Jan 2023 13:29
Operator : JC/MD
Sample : 01139-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH1Z9

Quant Time: Jan 13 22:26:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 11 00:53:59 2023
Response via : Initial Calibration

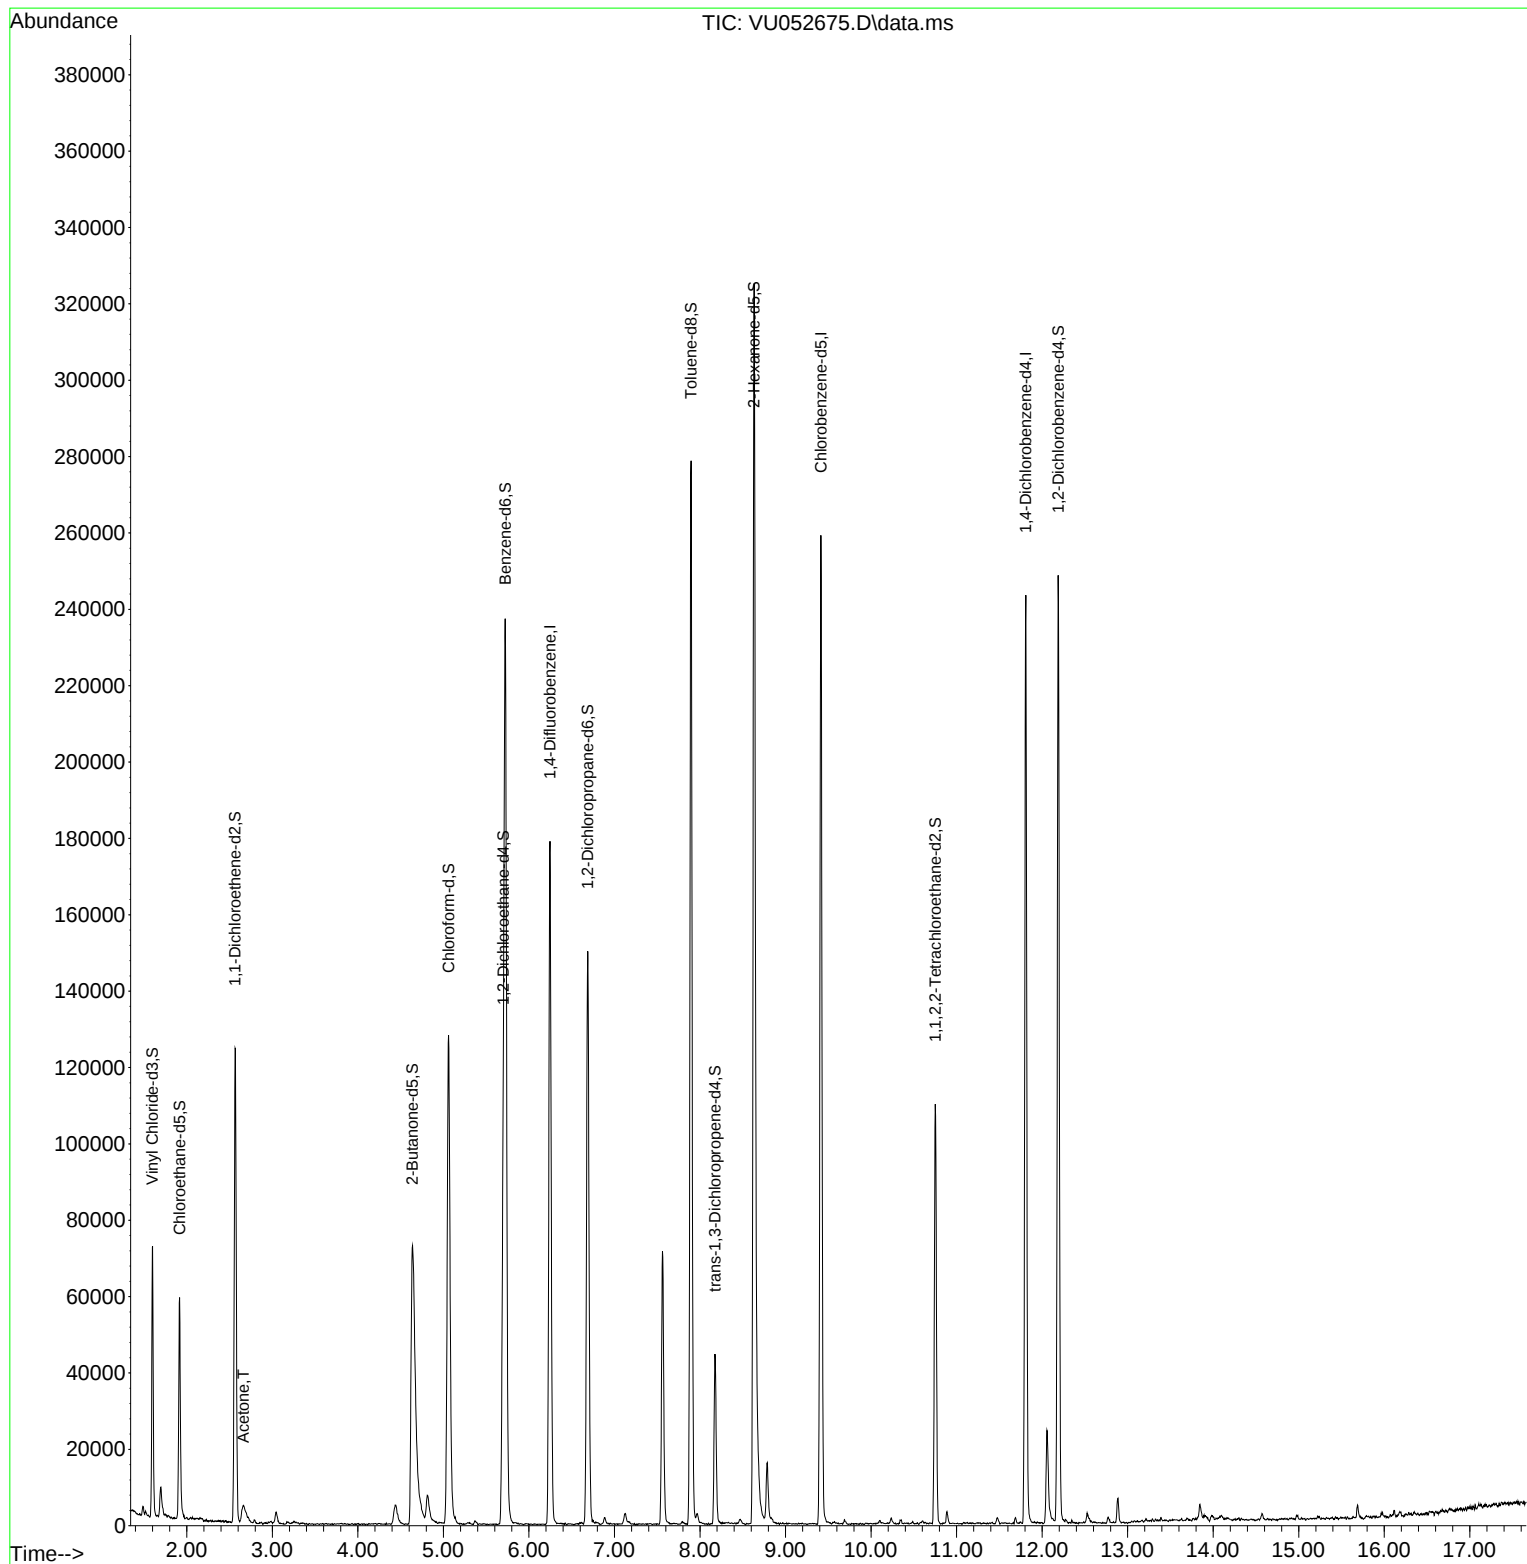

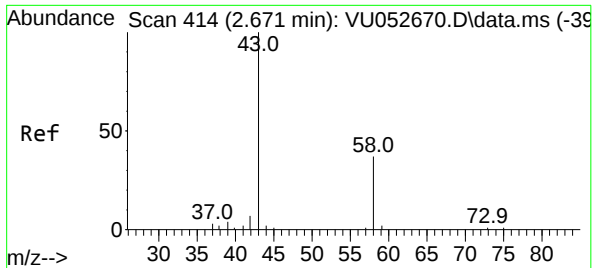

#13
 Acetone
 Concen: 5.025 ug/L
 RT: 2.661 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: VU052675.D
 Acq: 13 Jan 2023 13:29

Instrument :
 MSVOA_U
 ClientSampleId :
 BH1Z9

Tgt Ion: 43 Resp: 11971
 Ion Ratio Lower Upper
 43 100
 58 27.5 0.0 68.8

