

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011323\
 Data File : VU052692.D
 Acq On : 13 Jan 2023 20:08
 Operator : JC/MD
 Sample : VIBLK142
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK142

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU052678.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	72	81	91	rBV	62522	73626	11.96%	1.592%
2	1.916	170	179	194	rBV	55140	76661	12.46%	1.658%
3	2.565	365	381	397	rBV	118656	194394	31.59%	4.204%
4	3.591	690	700	712	rVB6	3887	8181	1.33%	0.177%
5	4.642	1012	1027	1063	rBV	65954	243101	39.50%	5.257%
6	5.060	1137	1157	1178	rBV	115447	257416	41.83%	5.566%
7	5.382	1249	1257	1273	rVB5	4696	9515	1.55%	0.206%
8	5.723	1341	1363	1389	rBV2	227889	592299	96.25%	12.808%
9	6.247	1512	1526	1544	rBV	165855	314844	51.16%	6.808%
10	6.687	1648	1663	1682	rBV	147840	286835	46.61%	6.202%
11	7.562	1923	1935	1951	rBV2	66277	116729	18.97%	2.524%
12	7.896	2025	2039	2054	rBV	259285	449803	73.09%	9.726%
13	8.176	2115	2126	2142	rBV2	40929	70854	11.51%	1.532%
14	8.633	2255	2268	2304	rBV2	320762	615386	100.00%	13.307%
15	9.414	2499	2511	2529	rBV	240608	392549	63.79%	8.488%
16	10.751	2915	2927	2942	rVB	105766	169468	27.54%	3.665%
17	11.806	3244	3255	3272	rBV	226100	356417	57.92%	7.707%
18	12.189	3359	3374	3395	rBV	241881	389322	63.26%	8.419%
19	12.890	3584	3592	3600	rVB4	5030	7167	1.16%	0.155%




Sum of corrected areas: 4624567

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011323\
Data File : VU052692.D
Acq On : 13 Jan 2023 20:08
Operator : JC/MD
Sample : VIBLK142
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK142

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

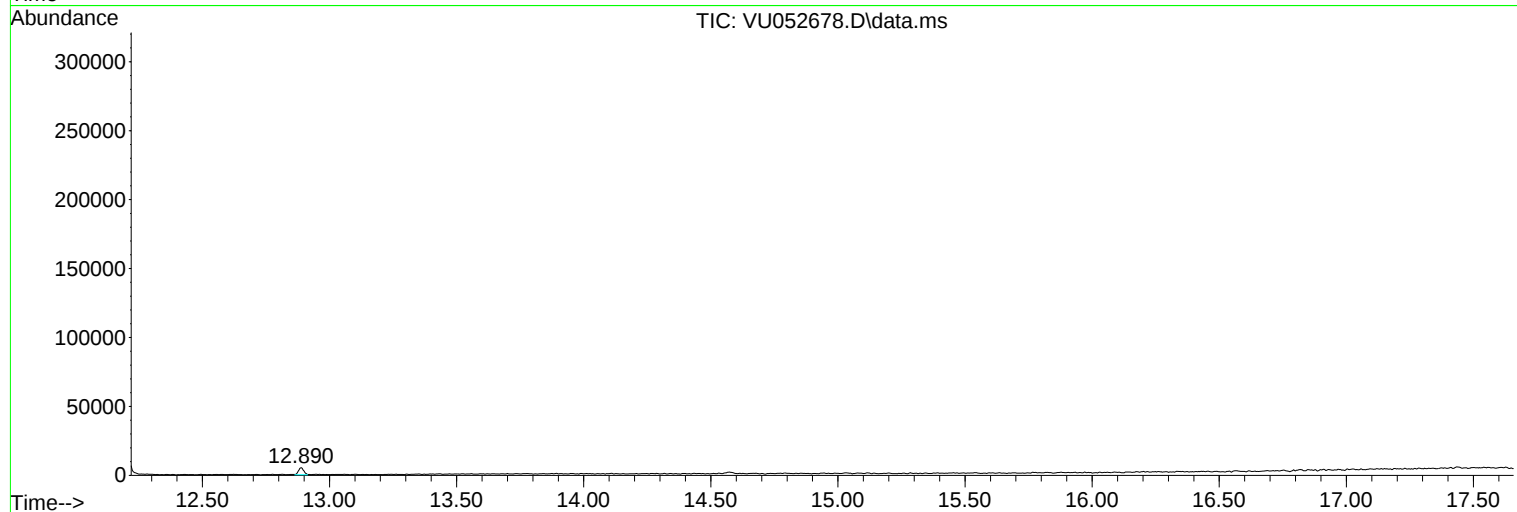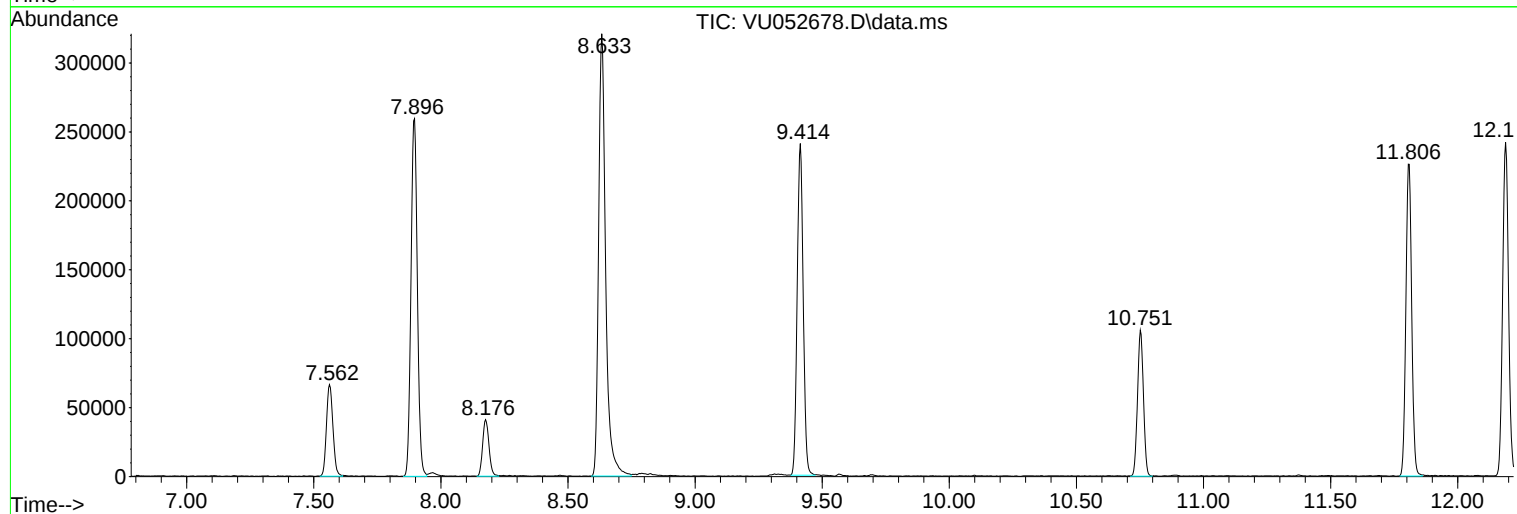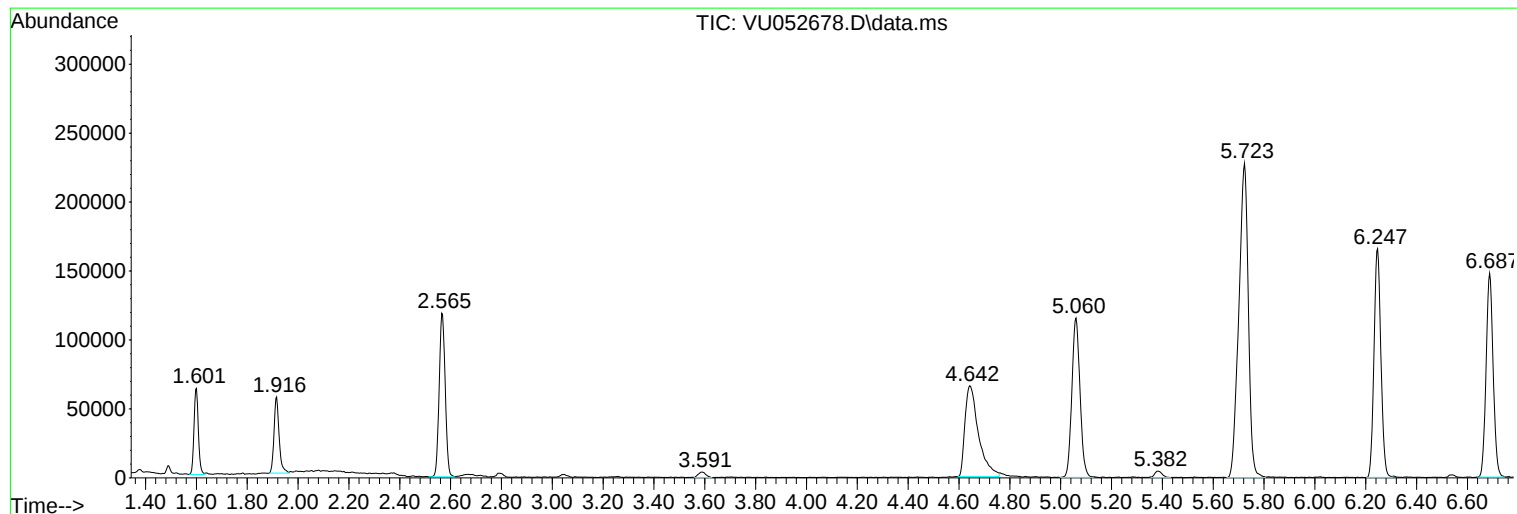

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011323\
Data File : VU052692.D
Acq On : 13 Jan 2023 20:08
Operator : JC/MD
Sample : VIBLK142
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK142

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011323\
Data File : VU052692.D
Acq On : 13 Jan 2023 20:08
Operator : JC/MD
Sample : VIBLK142
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK142

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------