
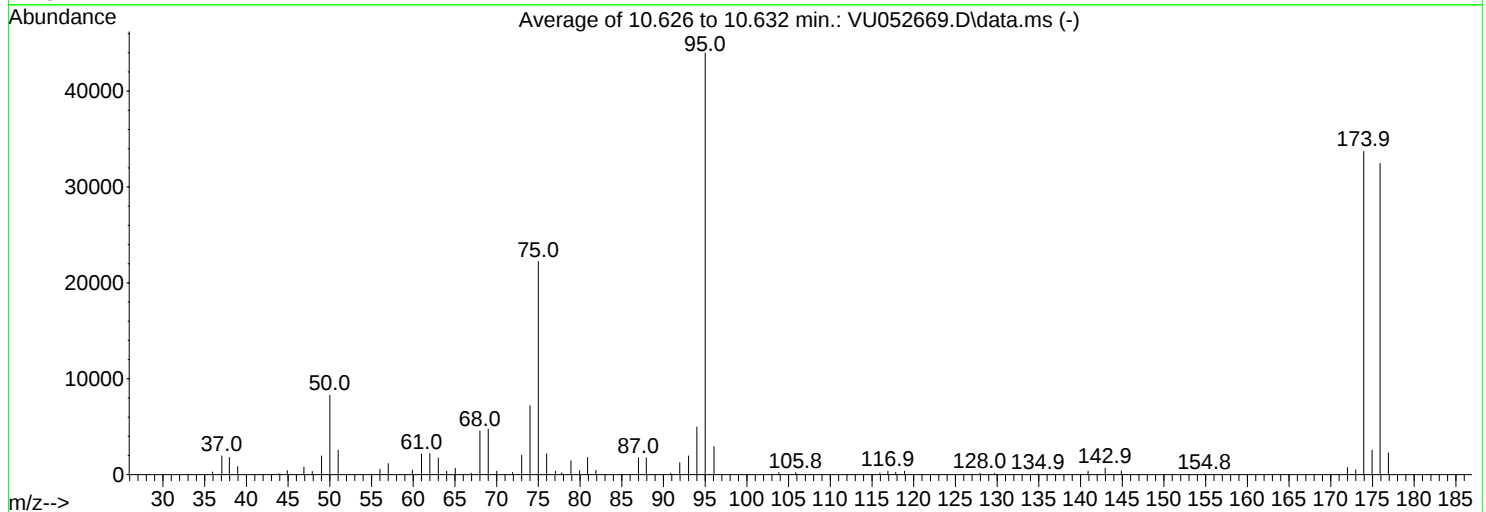


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011323\
 Data File : VU052669.D
 Acq On : 13 Jan 2023 09:15
 Operator : JC/MD
 Sample : BFB189
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB189

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Jan 11 00:53:59 2023

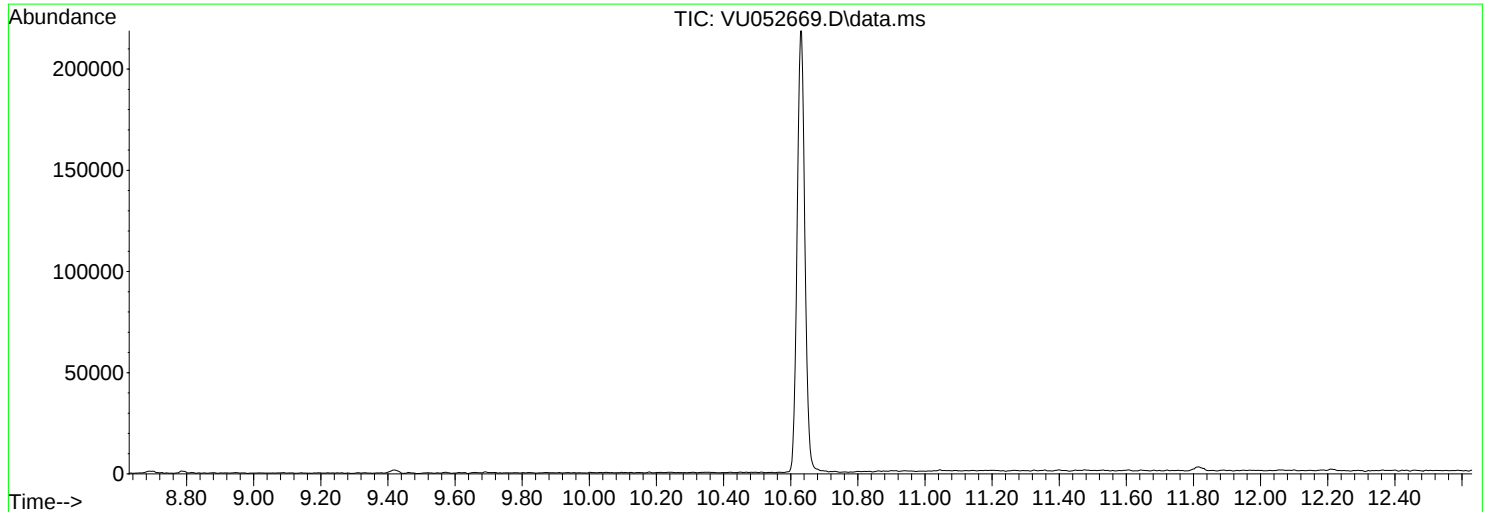

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	8270	PASS
75	95	30	80	50.5	22227	PASS
95	95	100	100	100.0	43995	PASS
96	95	5	9	6.7	2946	PASS
173	174	0.00	2	1.5	497	PASS
174	95	50	120	76.6	33715	PASS
175	174	5	9	7.6	2546	PASS
176	174	95	101	96.3	32467	PASS
177	176	5	9	7.0	2268	PASS

m/z	Abundance
35.90	215.0
37.90	103.0
39.80	167.0
44.00	440.0

Instrument :
MSVOA_U
ClientSampleId :
BFB189

m/z	Abundance
36.00	467.0
37.10	1891.0
38.00	1784.0
39.00	878.0
39.90	181.0
43.80	526.0
44.90	388.0
46.90	798.0
47.90	291.0
49.00	1749.0
50.00	8043.0
51.00	2604.0
56.00	552.0
56.90	1087.0
59.90	481.0
61.00	2062.0
62.00	2161.0
63.00	1776.0
64.00	313.0
65.10	636.0
67.00	169.0
68.00	4232.0
69.00	4444.0
70.00	346.0
71.80	198.0
73.00	2003.0
74.00	6878.0
75.00	20536.0
76.00	2255.0
77.10	344.0
77.80	216.0
78.90	1332.0
80.00	446.0
80.90	1758.0
81.90	408.0
87.00	1922.0
87.90	1677.0
90.90	106.0
91.90	1154.0
93.00	1797.0
94.00	4537.0
95.00	41616.0
96.00	3049.0
103.80	188.0
105.90	235.0
116.00	157.0
116.90	296.0
117.90	278.0
118.90	333.0
128.00	122.0
129.70	140.0
140.90	353.0
143.00	623.0
144.90	393.0
154.80	110.0
172.00	595.0
173.00	490.0
174.00	31392.0
174.90	2519.0
175.90	29656.0
176.90	2097.0

Instrument :
MSVOA_U
ClientSampleId :
BFB189

m/z	Abundance
36.00	475.0
37.10	2070.0
38.00	1925.0
38.90	851.0
39.90	209.0
43.90	560.0
44.90	422.0
46.90	831.0
47.90	362.0
49.00	2001.0
50.00	8571.0
51.00	2646.0
55.00	109.0
56.00	578.0
57.00	1182.0
59.90	489.0
61.00	2247.0
62.00	2231.0
63.00	1761.0
64.00	376.0
65.00	658.0
66.90	153.0
68.00	4722.0
69.00	4873.0
70.00	384.0
71.90	206.0
73.00	2133.0
74.00	7392.0
75.00	22856.0
76.00	2303.0
77.10	378.0
77.80	196.0
78.90	1493.0
80.00	418.0
80.90	1810.0
81.90	452.0
87.00	1772.0
88.00	1782.0
90.80	141.0
92.00	1309.0
93.00	1995.0
94.00	5174.0
95.00	45376.0
96.10	3071.0
103.80	222.0
105.90	227.0
115.90	161.0
116.90	358.0
117.80	254.0
118.90	369.0
128.00	162.0
129.70	143.0
134.90	121.0
140.90	351.0
142.90	682.0
144.90	384.0
172.00	771.0
173.00	515.0
173.90	34768.0
174.90	2597.0
175.90	33376.0
176.90	2382.0

Instrument :
MSVOA_U
ClientSampleId :
BFB189

m/z	Abundance
36.00	536.0
37.00	1914.0
38.00	1973.0
38.90	775.0
39.90	209.0
43.90	558.0
44.90	430.0
46.90	757.0
47.90	353.0
49.00	2107.0
50.00	8197.0
51.00	2415.0
52.00	142.0
55.00	127.0
56.00	533.0
57.10	1170.0
59.90	446.0
61.00	2186.0
62.00	2176.0
63.00	1650.0
64.00	385.0
65.00	694.0
66.90	133.0
68.00	4721.0
69.00	4930.0
70.00	361.0
72.00	248.0
73.00	1931.0
74.00	7359.0
75.00	23288.0
76.00	1954.0
77.00	351.0
77.80	165.0
78.90	1557.0
79.90	397.0
80.90	1778.0
81.90	474.0
87.00	1634.0
88.00	1818.0
90.80	181.0
92.00	1294.0
93.00	2072.0
94.00	5222.0
95.00	44992.0
96.10	2719.0
103.90	240.0
105.80	201.0
115.90	193.0
116.90	410.0
117.80	220.0
118.90	339.0
127.90	193.0
129.70	101.0
134.90	142.0
136.80	110.0
140.90	359.0
142.90	742.0
144.90	366.0
154.90	106.0
156.80	111.0
171.00	100.0
172.00	827.0
173.00	486.0
173.90	34984.0
175.00	2523.0
175.90	34368.0
176.90	2326.0

Instrument :
MSVOA_U
ClientSampleId :
BFB189