

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011325\
 Data File : VU062712.D
 Acq On : 13 Jan 2025 13:06
 Operator : MD/SY
 Sample : Q1059-16
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHSL7

Quant Time: Jan 13 19:01:47 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jan 13 18:58:58 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	87809	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	82945	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	39063	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	20139	4.141	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.800%
7) Chloroethane-d5	1.904	69	18547	4.741	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.800%
11) 1,1-Dichloroethene-d2	2.557	65	10515	4.174	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.400%
20) 2-Butanone-d5	4.605	46	53013	53.336	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.680%
24) Chloroform-d	5.049	84	59271	4.954	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.000%
26) 1,2-Dichloroethane-d4	5.689	65	33215	5.118	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.400%
32) Benzene-d6	5.714	84	98045	4.836	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.800%
36) 1,2-Dichloropropane-d6	6.679	67	28558	5.080	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.600%
41) Toluene-d8	7.888	98	89234	4.517	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.400%
43) trans-1,3-Dichloroprop...	8.174	79	11756	4.195	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.000%
46) 2-Hexanone-d5	8.621	63	43206	49.024	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.040%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	25088	5.329	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.600%
66) 1,2-Dichlorobenzene-d4	12.187	152	33249	5.116	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.400%
Target Compounds					Qvalue	
25) Chloroform	5.075	83	6492	0.505	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011325\
Data File : VU062712.D
Acq On : 13 Jan 2025 13:06
Operator : MD/SY
Sample : Q1059-16
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHSL7

Quant Time: Jan 13 19:01:47 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jan 13 18:58:58 2025
Response via : Initial Calibration

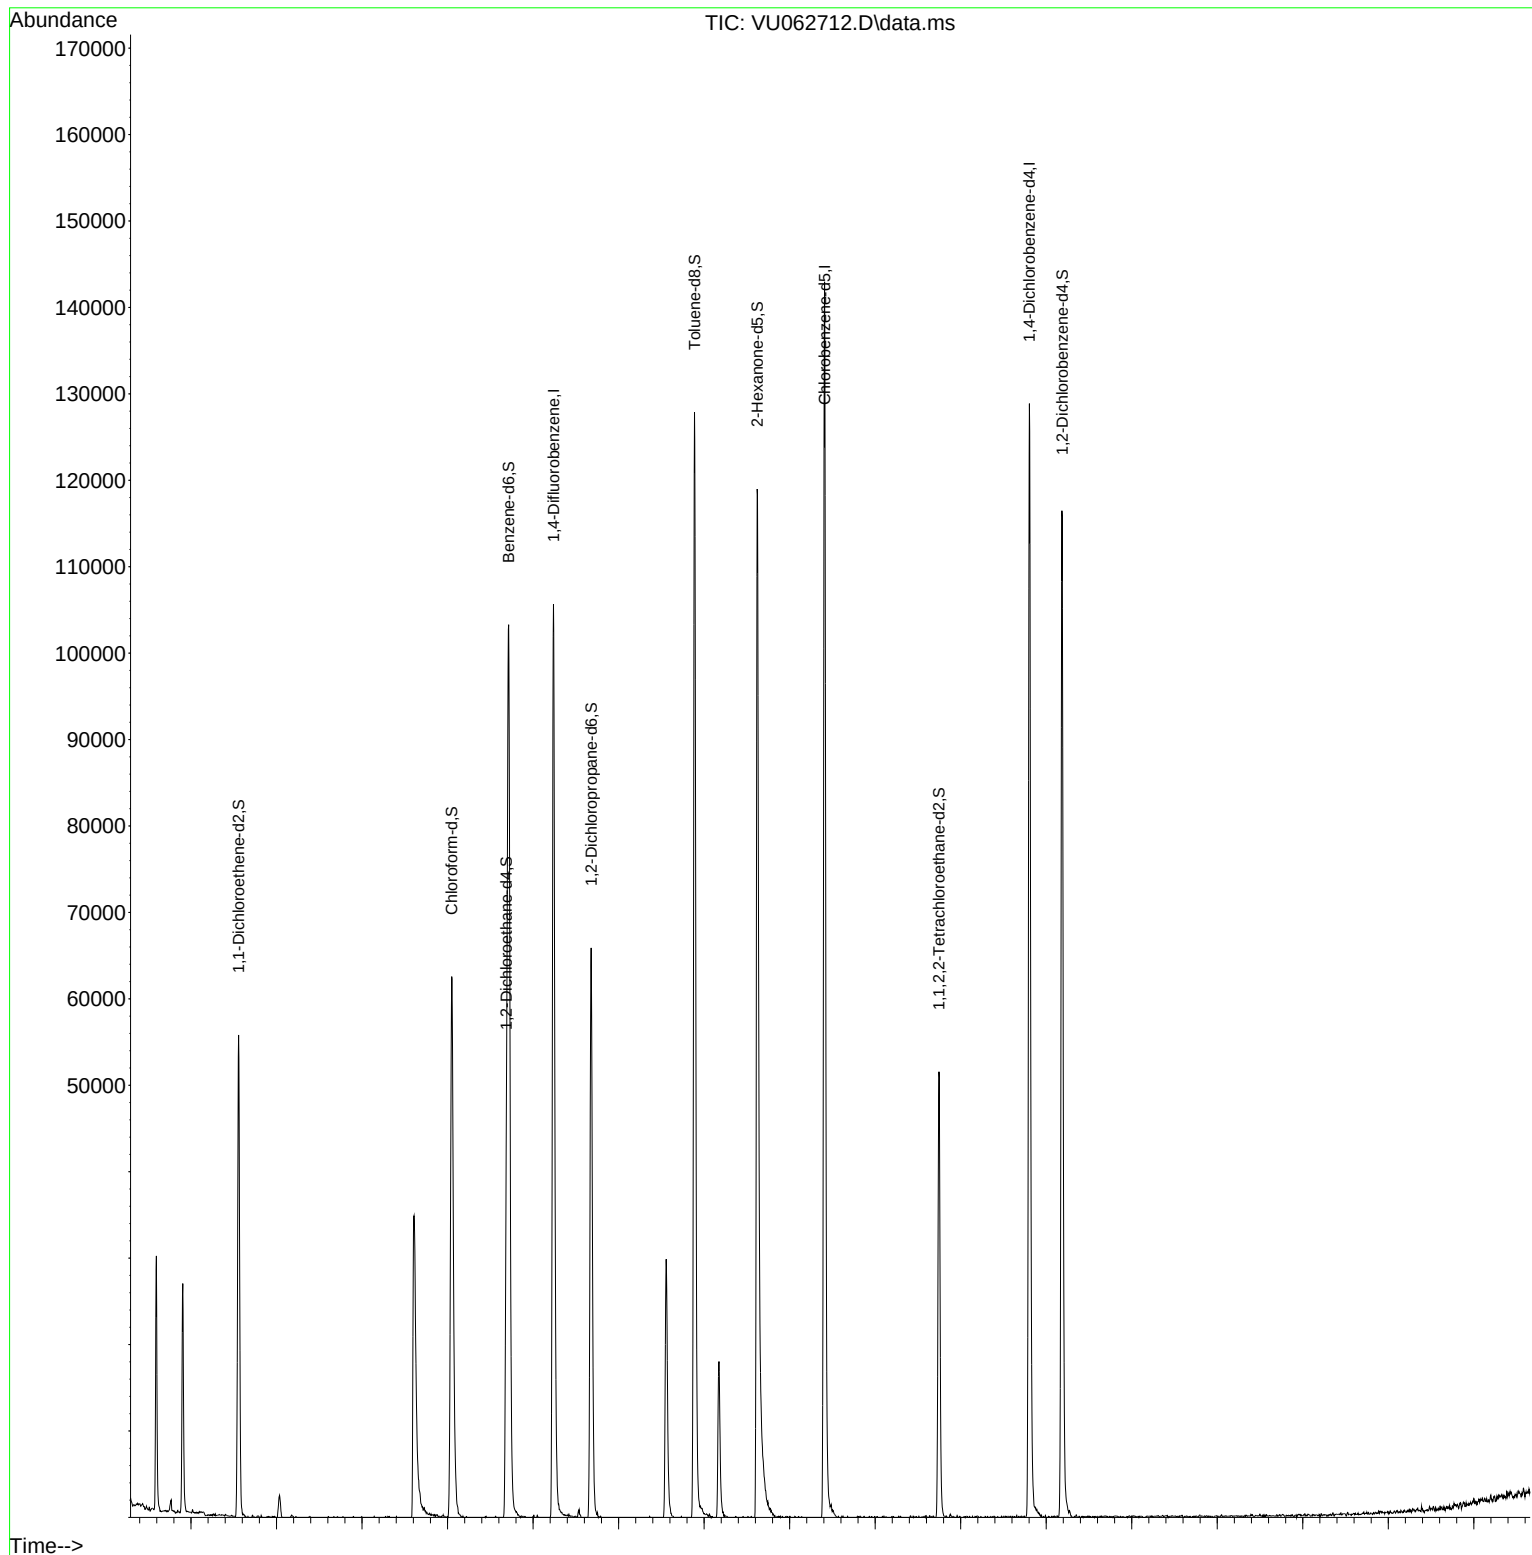

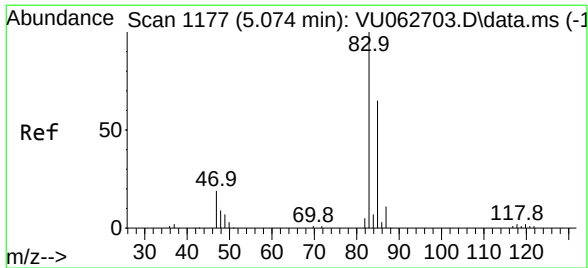

#25
 Chloroform
 Concen: 0.505 ug/L
 RT: 5.075 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VU062712.D
 Acq: 13 Jan 2025 13:06

Instrument :
 MSVOA_U
 ClientSampleId :
 BHSL7

Tgt Ion: 83 Resp: 6492
 Ion Ratio Lower Upper
 83 100
 85 69.4 45.8 85.2

