

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011325\
 Data File : VU062713.D
 Acq On : 13 Jan 2025 13:30
 Operator : MD/SY
 Sample : Q1059-17
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHSL8

Quant Time: Jan 13 19:02:01 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jan 13 18:58:58 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	90792	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	84250	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	38385	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	20281	4.033	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.600%
7) Chloroethane-d5	1.904	69	18861	4.663	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.200%
11) 1,1-Dichloroethene-d2	2.557	65	11458	4.399	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.000%
20) 2-Butanone-d5	4.605	46	55828	54.323	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.640%
24) Chloroform-d	5.049	84	61493	4.970	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.400%
26) 1,2-Dichloroethane-d4	5.689	65	36791	5.483	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.600%
32) Benzene-d6	5.714	84	102819	4.993	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.800%
36) 1,2-Dichloropropane-d6	6.679	67	30079	5.268	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.400%
41) Toluene-d8	7.888	98	93862	4.678	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.600%
43) trans-1,3-Dichloroprop...	8.171	79	12893	4.530	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.600%
46) 2-Hexanone-d5	8.621	63	43275	48.342	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.680%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	25521	5.337	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.800%
66) 1,2-Dichlorobenzene-d4	12.183	152	34659	5.427	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.600%
Target Compounds					Qvalue	
25) Chloroform	5.078	83	5885	0.443	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011325\
Data File : VU062713.D
Acq On : 13 Jan 2025 13:30
Operator : MD/SY
Sample : Q1059-17
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHSL8

Quant Time: Jan 13 19:02:01 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jan 13 18:58:58 2025
Response via : Initial Calibration

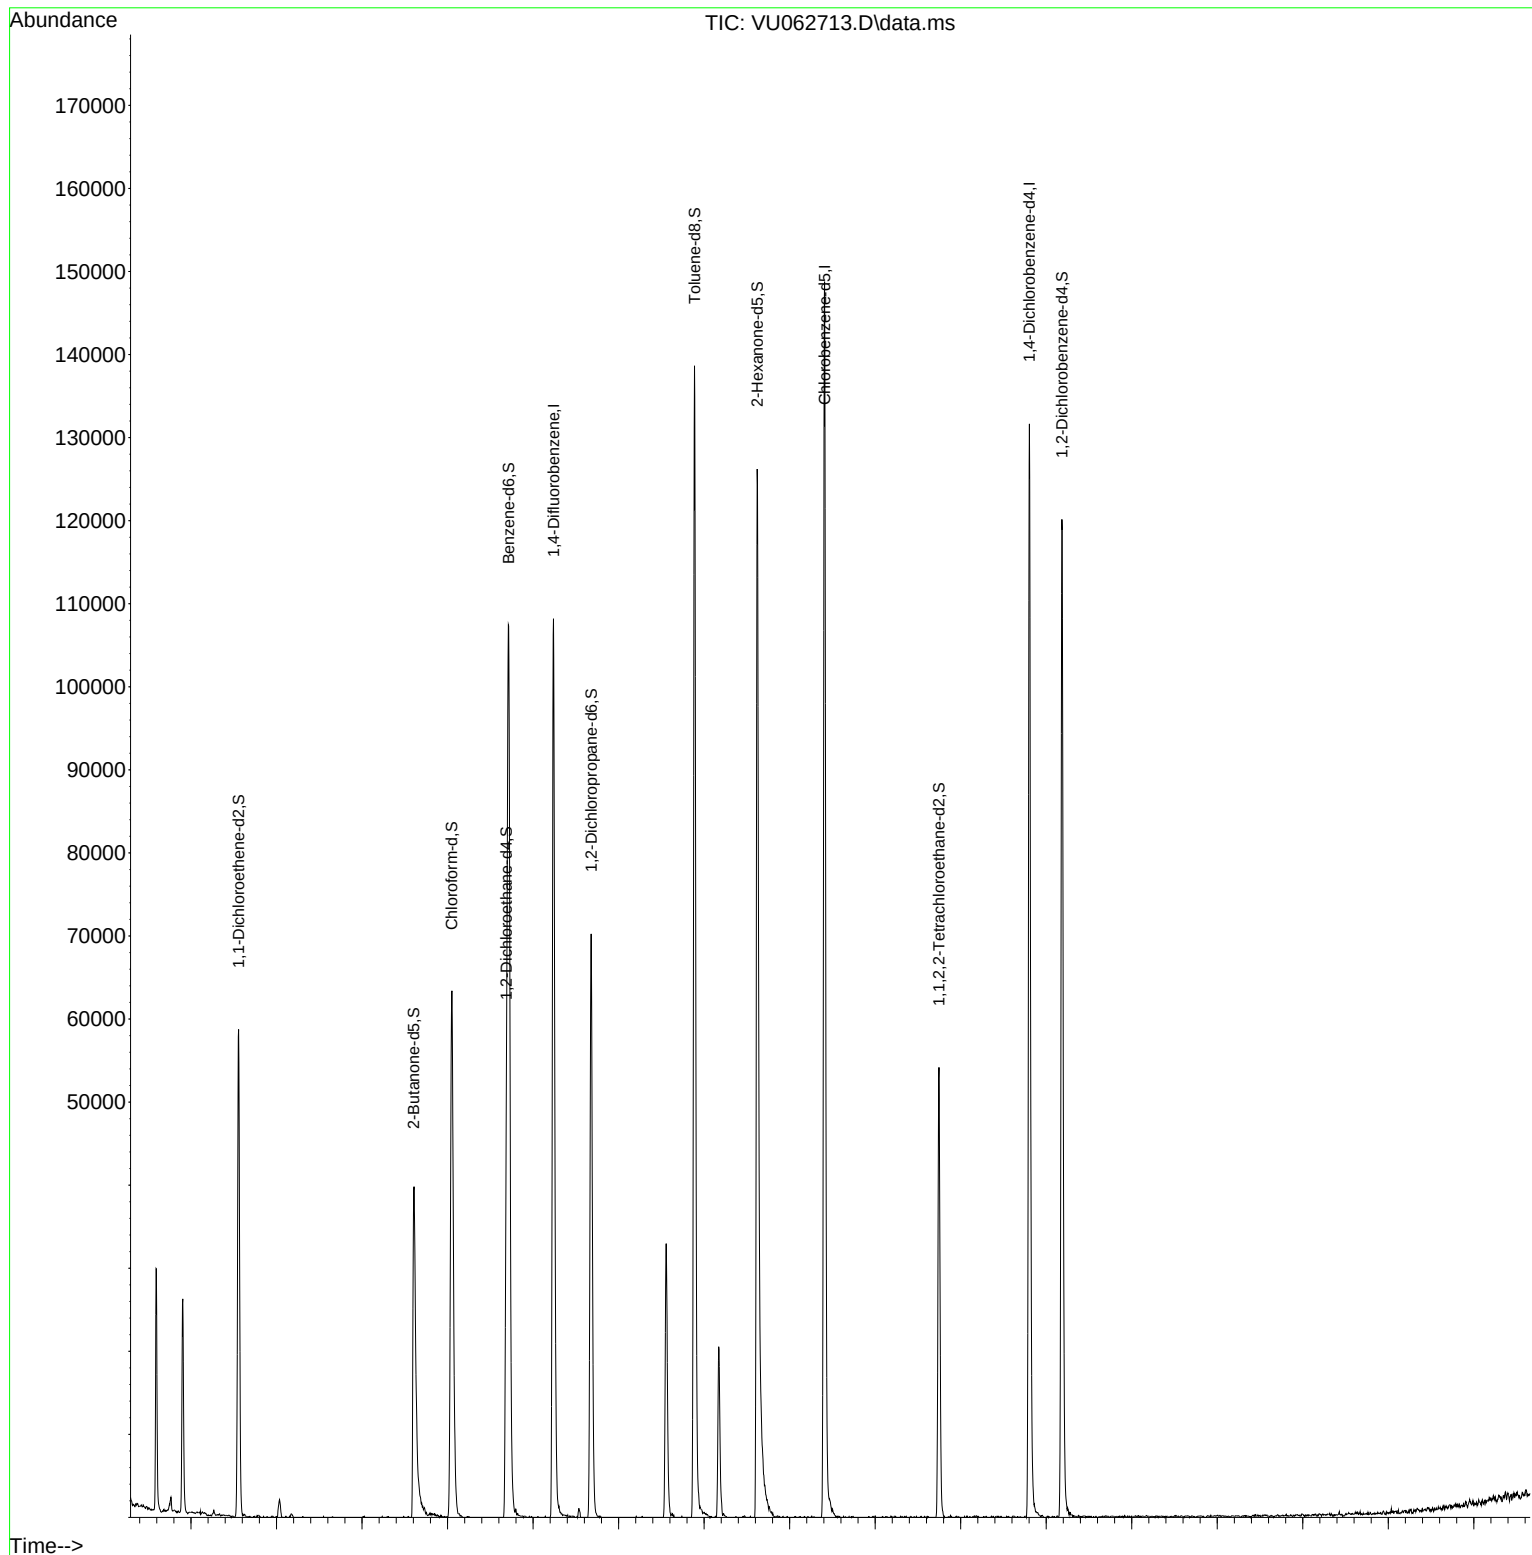

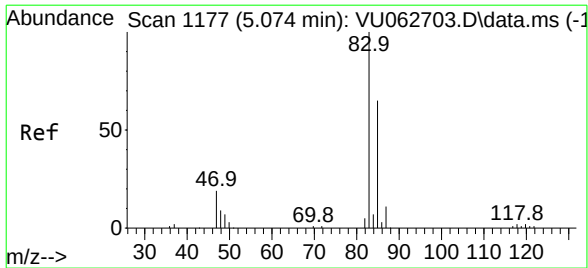

#25
 Chloroform
 Concen: 0.443 ug/L
 RT: 5.078 min Scan# 1178
 Delta R.T. 0.003 min
 Lab File: VU062713.D
 Acq: 13 Jan 2025 13:30

Instrument :
 MSVOA_U
 ClientSampleId :
 BHSL8

Tgt Ion: 83 Resp: 5885
 Ion Ratio Lower Upper
 83 100
 85 61.3 45.8 85.2

