

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011325\
 Data File : VU062715.D
 Acq On : 13 Jan 2025 14:19
 Operator : MD/SY
 Sample : Q1059-19
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHSM1

Quant Time: Jan 13 19:02:34 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jan 13 18:58:58 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	90958	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	84761	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	38304	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	19150	3.801	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.000%
7) Chloroethane-d5	1.904	69	17338	4.278	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.600%
11) 1,1-Dichloroethene-d2	2.557	65	10591	4.058	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.200%
20) 2-Butanone-d5	4.608	46	51520	50.039	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.080%
24) Chloroform-d	5.052	84	58862	4.749	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.000%
26) 1,2-Dichloroethane-d4	5.688	65	35042	5.212	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.200%
32) Benzene-d6	5.714	84	99250	4.790	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.800%
36) 1,2-Dichloropropane-d6	6.679	67	28824	5.018	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.400%
41) Toluene-d8	7.888	98	89526	4.435	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.800%
43) trans-1,3-Dichloroprop...	8.174	79	11353	3.965	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.200%
46) 2-Hexanone-d5	8.621	63	40436	44.898	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.800%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	23978	4.984	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.600%
66) 1,2-Dichlorobenzene-d4	12.187	152	33660	5.282	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.600%
Target Compounds						
13) Acetone	2.615	43	8354	10.243	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011325\
Data File : VU062715.D
Acq On : 13 Jan 2025 14:19
Operator : MD/SY
Sample : Q1059-19
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHSM1

Quant Time: Jan 13 19:02:34 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jan 13 18:58:58 2025
Response via : Initial Calibration

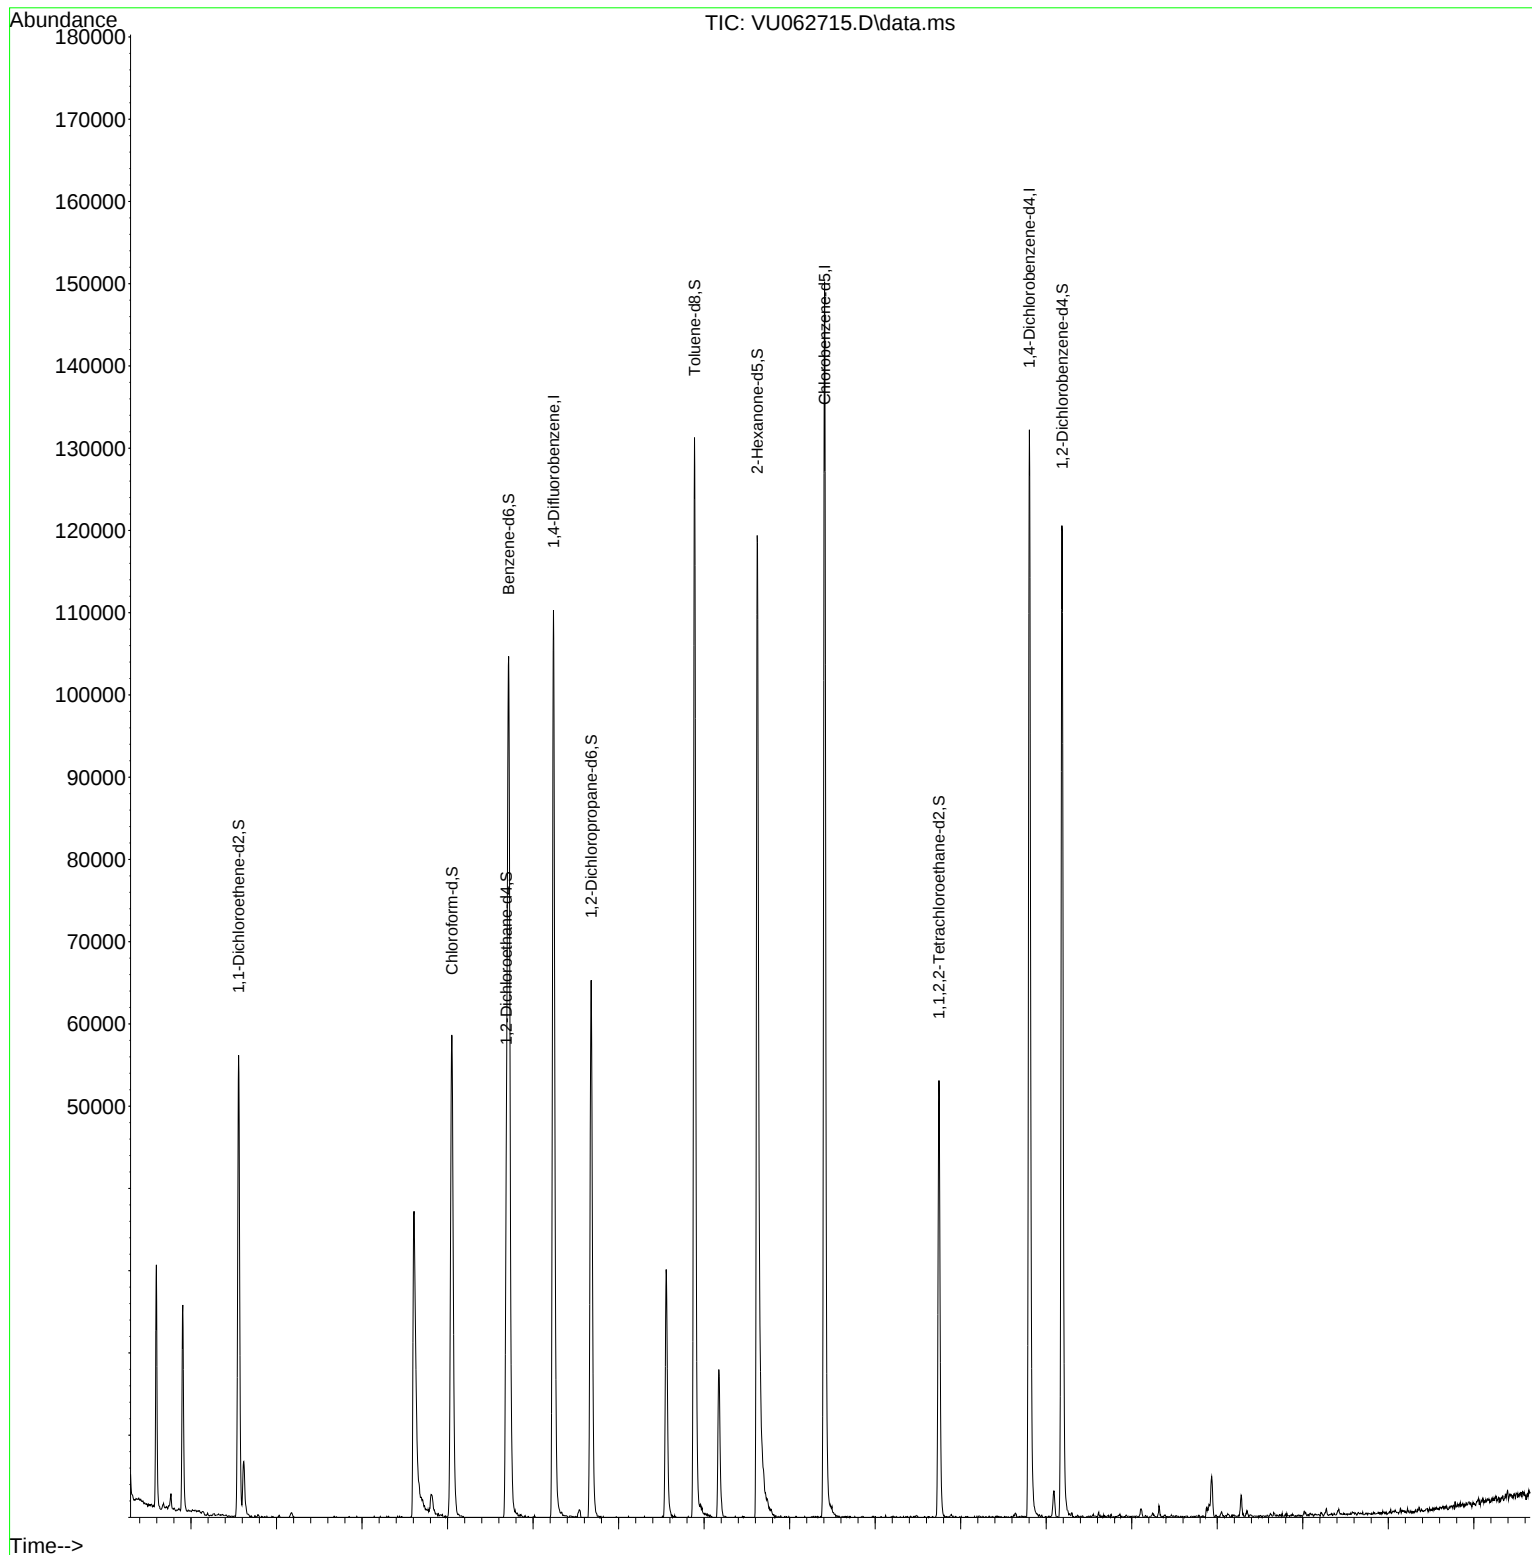

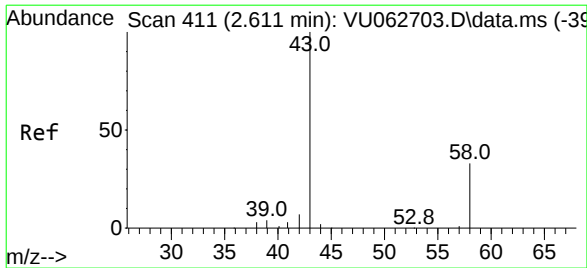

#13

Acetone

Concen: 10.243 ug/L

RT: 2.615 min Scan# 41

Delta R.T. 0.003 min

Lab File: VU062715.D


Acq: 13 Jan 2025 14:19

Instrument :

MSVOA_U

ClientSampleId :

BHSM1

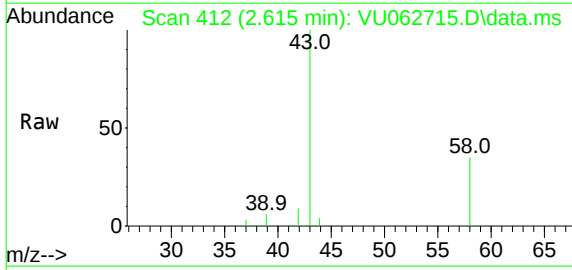

Tgt Ion: 43 Resp: 8354

Ion Ratio Lower Upper

43 100

58 31.4 0.0 64.4

