

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011325\
 Data File : VU062723.D
 Acq On : 13 Jan 2025 17:37
 Operator : MD/SY
 Sample : Q1058-07DL 5X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH8X6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU062723.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.461	46	53	70	rBV	22375	41736	14.58%	1.453%
2	1.567	74	86	87	rVV2	9354	18229	6.37%	0.635%
3	1.596	89	95	115	rVB2	35703	55346	19.34%	1.927%
4	1.901	184	190	213	rVB	27205	43214	15.10%	1.504%
5	2.567	382	397	421	rBV4	130762	256433	89.61%	8.928%
6	3.171	574	585	601	rVB3	5919	13110	4.58%	0.456%
7	3.856	785	798	816	rBB3	9721	22603	7.90%	0.787%
8	4.608	1023	1032	1039	rBV	40878	86161	30.11%	3.000%
9	5.049	1155	1169	1189	rBV	60627	135715	47.43%	4.725%
10	5.711	1357	1375	1403	rBV2	107433	286167	100.00%	9.963%
11	6.239	1527	1539	1572	rBV	113658	219447	76.68%	7.640%
12	6.531	1619	1630	1652	rBV2	68171	128036	44.74%	4.458%
13	6.679	1664	1676	1702	rBB2	66530	131329	45.89%	4.572%
14	7.557	1938	1949	1964	rBV2	35282	62512	21.84%	2.176%
15	7.888	2041	2052	2071	rBV	135763	236979	82.81%	8.250%
16	8.171	2131	2140	2156	rBV2	21300	36438	12.73%	1.269%
17	8.621	2270	2280	2318	rBV	139532	271789	94.98%	9.462%
18	9.409	2514	2525	2556	rBV	160209	268025	93.66%	9.331%
19	10.746	2930	2941	2960	rBB	57368	92881	32.46%	3.234%
20	11.804	3259	3270	3296	rBV	147214	246122	86.01%	8.569%
21	12.184	3377	3388	3408	rBV	130639	220050	76.90%	7.661%




Sum of corrected areas: 2872322

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011325\
Data File : VU062723.D
Acq On : 13 Jan 2025 17:37
Operator : MD/SY
Sample : Q1058-07DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH8X6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

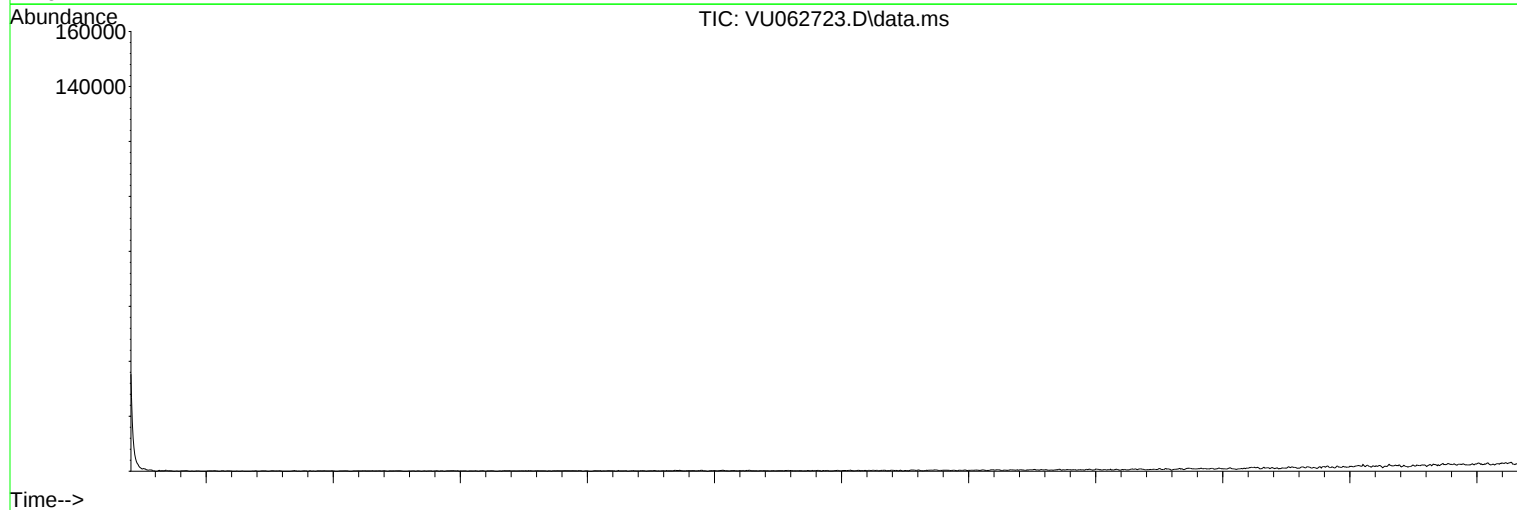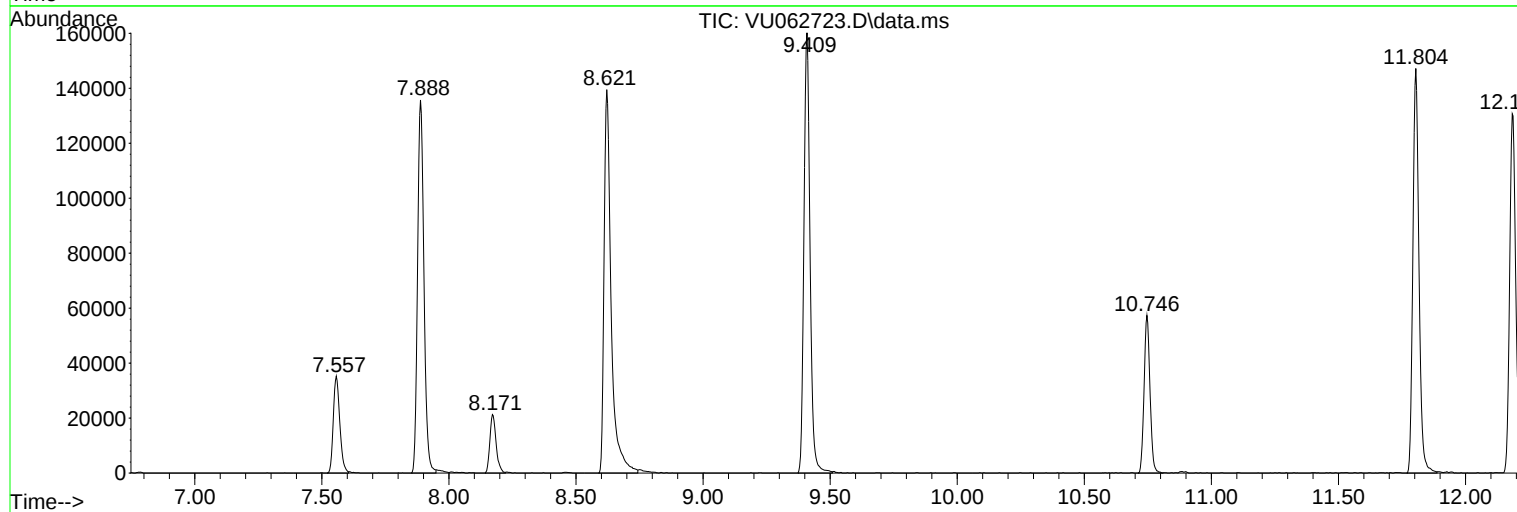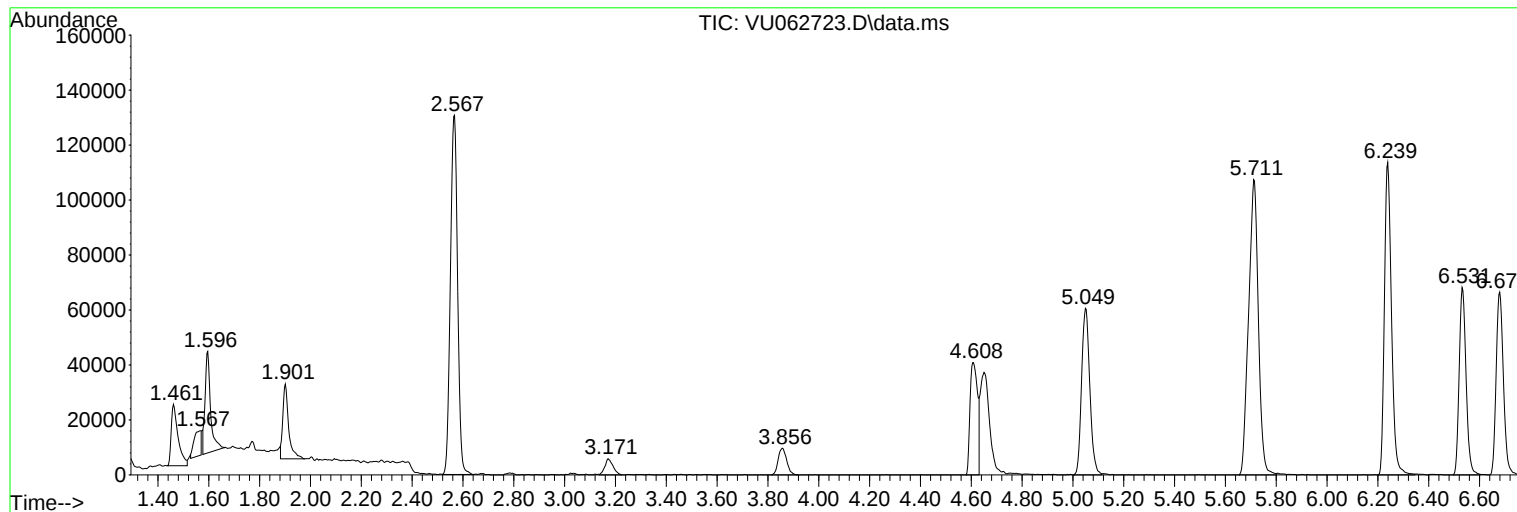

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011325\
Data File : VU062723.D
Acq On : 13 Jan 2025 17:37
Operator : MD/SY
Sample : Q1058-07DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH8X6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011325\
Data File : VU062723.D
Acq On : 13 Jan 2025 17:37
Operator : MD/SY
Sample : Q1058-07DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH8X6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc