
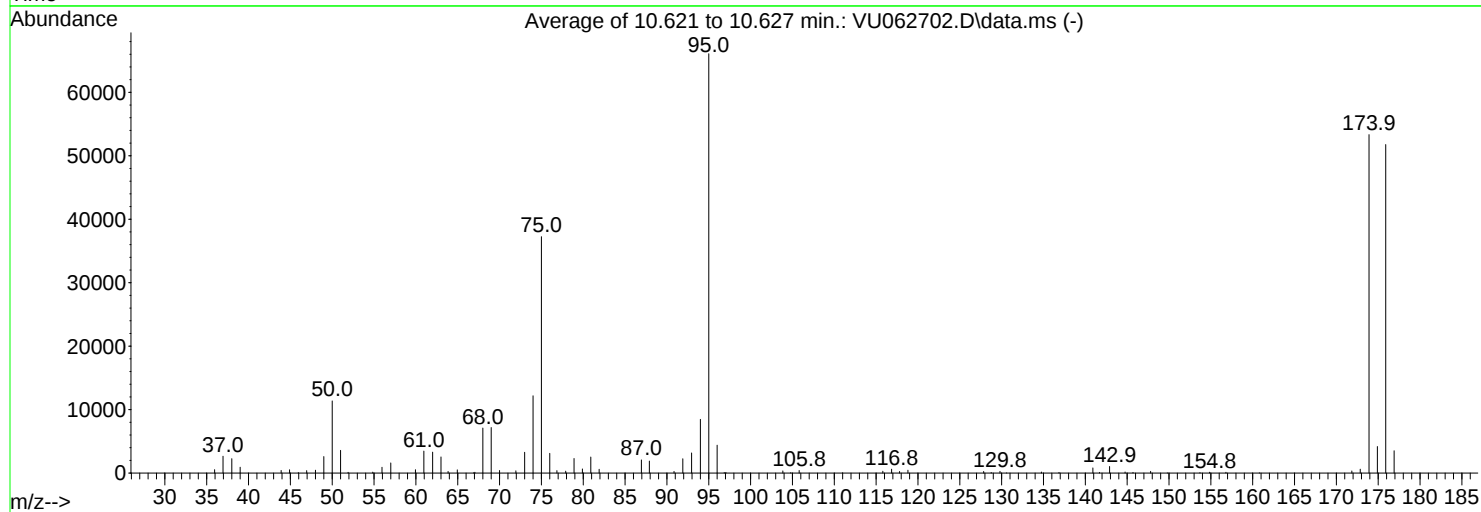


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011325\
Data File : VU062702.D
Acq On : 13 Jan 2025 08:10
Operator : MD/SY
Sample : BFB059
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB059

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Jan 13 18:58:58 2025

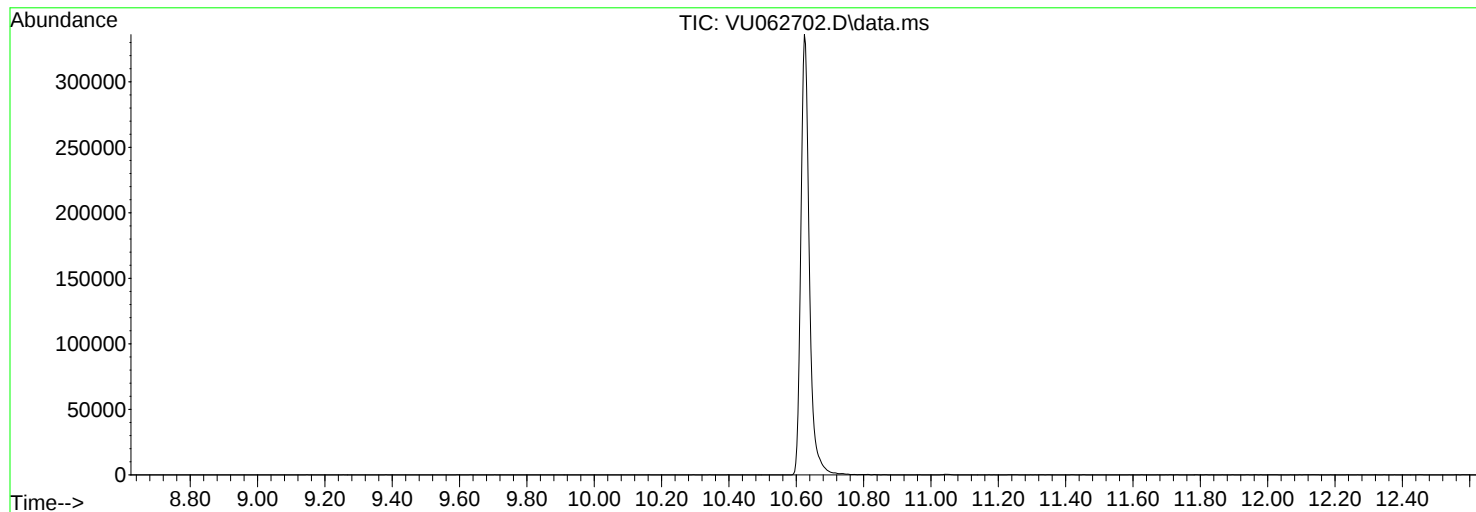

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	11372	PASS
75	95	30	80	56.4	37259	PASS
95	95	100	100	100.0	66085	PASS
96	95	5	9	6.6	4394	PASS
173	174	0.00	2	1.2	619	PASS
174	95	50	120	80.7	53336	PASS
175	174	5	9	7.8	4180	PASS
176	174	95	101	97.1	51771	PASS
177	176	5	9	6.8	3520	PASS

m/z

Abundance

Instrument :

MSVOA_U

ClientSampleId :

BFB059

m/z	Abundance
36.00	508.0
37.00	2636.0
38.00	2142.0
39.00	863.0
43.90	417.0
44.90	528.0
47.00	391.0
48.00	402.0
49.00	2641.0
50.00	10793.0
51.00	3534.0
51.90	116.0
54.90	185.0
55.90	969.0
57.00	1665.0
60.00	493.0
60.90	3267.0
62.00	3097.0
63.00	2564.0
63.90	311.0
65.00	491.0
66.90	143.0
68.00	6618.0
69.00	7129.0
70.00	386.0
71.90	377.0
73.00	3181.0
74.00	11817.0
75.00	36256.0
76.00	2876.0
76.80	343.0
77.90	313.0
78.90	2265.0
79.90	650.0
80.90	2389.0
81.90	592.0
87.00	1917.0
87.90	1692.0
90.80	214.0
91.90	2341.0
93.00	3063.0
94.00	8045.0
95.00	64528.0
96.00	4314.0
96.80	118.0
103.80	336.0
104.80	106.0
105.80	388.0
115.70	294.0
116.90	569.0
117.80	253.0
118.80	472.0
127.80	270.0
128.80	100.0
129.80	305.0
134.80	176.0
140.90	736.0
141.70	115.0
142.90	986.0
144.70	167.0
145.70	104.0
147.80	256.0
149.80	101.0
154.80	141.0
156.80	128.0
171.80	306.0
172.90	553.0
173.90	49984.0
174.90	4059.0
175.90	49136.0
176.90	3366.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

m/z	Abundance
35.90	557.0
37.00	2729.0
38.00	2377.0
39.00	938.0
43.90	427.0
44.90	556.0
46.00	100.0
47.00	403.0
48.00	473.0
49.00	2695.0
50.00	11767.0
51.00	3694.0
51.90	125.0
54.80	146.0
55.90	932.0
57.00	1635.0
60.00	523.0
61.00	3600.0
62.00	3378.0
63.00	2578.0
63.80	251.0
65.00	551.0
67.10	176.0
68.00	7317.0
69.00	7440.0
70.00	423.0
71.90	371.0
73.00	3388.0
74.00	12551.0
75.00	38360.0
76.00	3217.0
76.90	386.0
77.90	317.0
78.90	2340.0
79.90	657.0
80.90	2605.0
81.90	635.0
86.90	2117.0
87.90	1927.0
90.90	271.0
91.90	2310.0
93.00	3279.0
94.00	8700.0
95.00	68232.0
96.00	4483.0
96.90	132.0
97.10	133.0
103.90	346.0
104.80	106.0
105.80	409.0
111.00	110.0
115.80	299.0
116.80	638.0
117.80	253.0
118.80	467.0
127.80	246.0
128.70	102.0
129.80	285.0
130.60	100.0
134.80	172.0
136.90	128.0
140.90	818.0
141.70	115.0
142.90	1064.0
144.80	176.0
145.70	107.0
147.80	298.0
153.70	114.0
154.80	148.0
156.80	143.0
171.90	338.0
172.80	629.0
173.90	54960.0
174.90	4285.0
175.90	53288.0
176.90	3638.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

m/z	Abundance
35.90	563.0
36.90	2611.0
38.00	2295.0
39.00	963.0
43.90	413.0
44.90	493.0
45.90	117.0
46.90	357.0
48.00	488.0
49.00	2486.0
50.00	11556.0
51.00	3516.0
51.90	141.0
54.80	124.0
56.00	840.0
57.00	1495.0
59.90	576.0
61.00	3541.0
62.00	3435.0
63.00	2484.0
63.90	221.0
64.90	471.0
67.00	219.0
68.00	7345.0
69.00	6976.0
70.00	432.0
72.00	328.0
73.00	3261.0
74.00	12172.0
75.00	37160.0
76.00	3234.0
76.90	423.0
77.90	278.0
78.90	2303.0
79.90	642.0
80.90	2577.0
81.90	562.0
86.90	2198.0
87.90	2047.0
90.90	329.0
91.90	2104.0
92.90	3174.0
94.00	8651.0
95.00	65496.0
96.00	4385.0
97.00	148.0
103.90	356.0
105.80	439.0
115.90	290.0
116.80	647.0
117.80	255.0
118.80	436.0
127.90	264.0
128.70	101.0
129.80	232.0
134.70	152.0
136.80	166.0
140.90	871.0
141.70	104.0
142.90	1059.0
144.80	190.0
145.70	107.0
147.80	272.0
153.70	120.0
154.90	136.0
156.80	126.0
160.80	117.0
171.90	361.0
172.80	676.0
173.90	55064.0
174.90	4196.0
175.90	52888.0
176.90	3557.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059