

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011421\
 Data File : VU042023.D
 Acq On : 14 Jan 2021 10:33
 Operator : SY/MD
 Sample : VU0114WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK21

Quant Time: Jan 15 05:21:15 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 15 05:20:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	141799	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	117666	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.809	152	50687	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	45049	4.21	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.20%
7) Chloroethane-d5	1.919	69	47286	4.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.40%
11) 1,1-Dichloroethene-d2	2.575	63	67424	3.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.60%
20) 2-Butanone-d5	4.652	46	164687	45.86	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.72%
24) Chloroform-d	5.076	84	93234	4.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.20%
26) 1,2-Dichloroethane-d4	5.713	65	52945	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.60%
32) Benzene-d6	5.739	84	178486	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.80%
36) 1,2-Dichloropropane-d6	6.700	67	65386	5.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.80%
41) Toluene-d8	7.903	98	135700	3.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.80%
43) trans-1,3-Dichloroprop...	8.182	79	21219	4.23	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.60%
46) 2-Hexanone-d5	8.642	63	120018	46.69	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.38%
57) 1,1,2,2-Tetrachloroeth...	10.755	84	46258	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.40%
64) 1,2-Dichlorobenzene-d4	12.189	152	47170	4.94	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.80%
Target Compounds						
16) Methylene chloride	3.057	84	3192	0.25	ug/L	Qvalue 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011421\
Data File : VU042023.D
Acq On : 14 Jan 2021 10:33
Operator : SY/MD
Sample : VU0114WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK21

Quant Time: Jan 15 05:21:15 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 15 05:20:45 2021
Response via : Initial Calibration

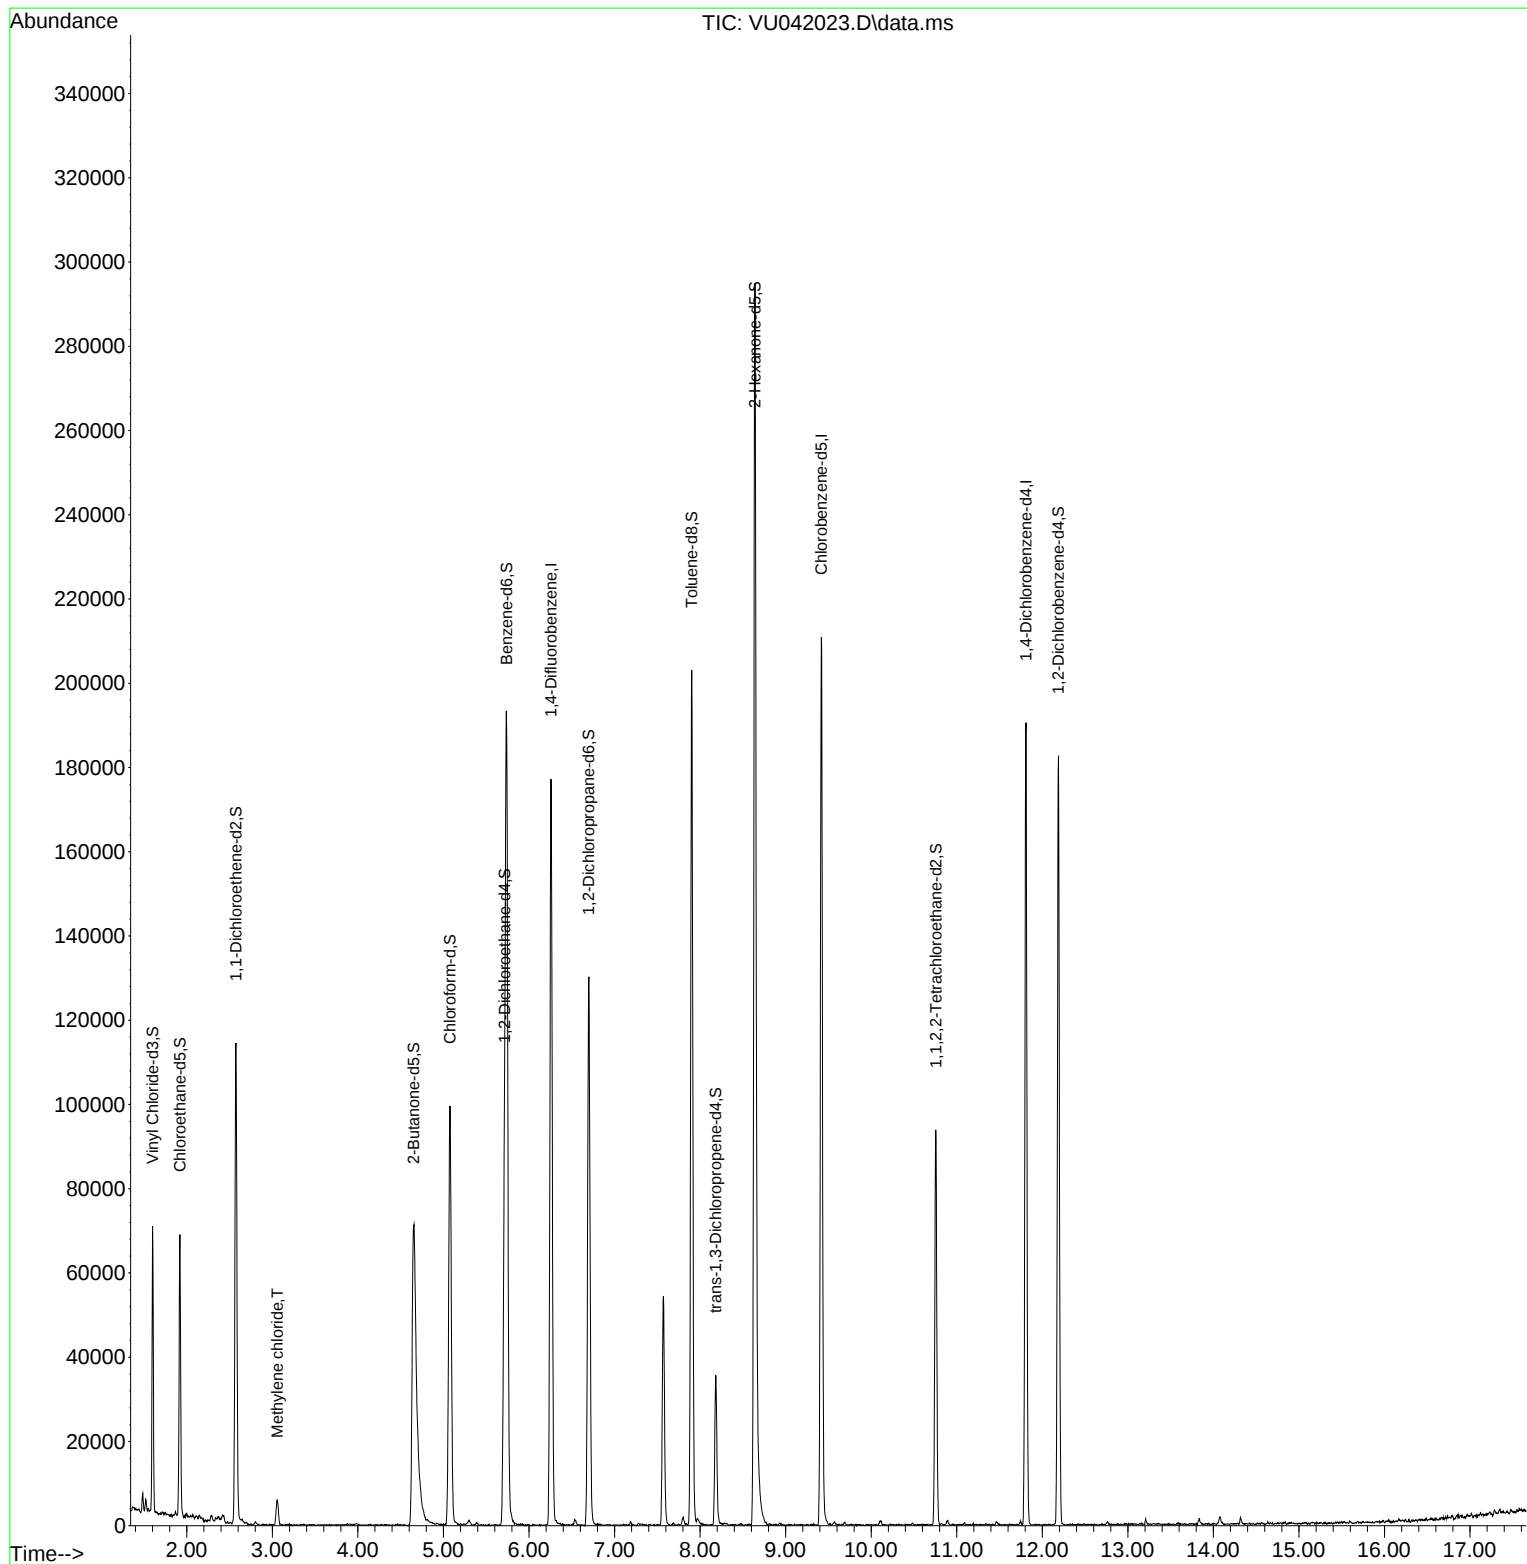

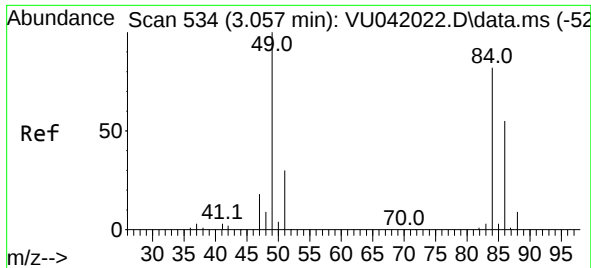

#16
Methylene chloride
Concen: 0.25 ug/L
RT: 3.057 min Scan# 534
Delta R.T. 0.000 min
Lab File: VU042023.D
Acq: 14 Jan 2021 10:33

Instrument :
MSVOA_U
ClientSampleId :
VBLK21

Tgt Ion:	84	Resp:	3192
Ion	Ratio	Lower	Upper
84	100		
86	50.6	42.6	79.0
49	91.5	86.2	160.0

