

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011421\
 Data File : VU042051.D
 Acq On : 14 Jan 2021 23:13
 Operator : SY/MD
 Sample : M1065-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXP1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC: VU042051.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	96	rVB	51702	56623	7.79%	1.266%
2	1.919	172	180	191	rVB	55821	68137	9.38%	1.524%
3	2.144	240	250	263	rVB2	8416	14070	1.94%	0.315%
4	2.575	372	384	401	rBV	93219	154848	21.31%	3.463%
5	3.199	565	578	592	rVB2	4365	9878	1.36%	0.221%
6	3.379	619	634	649	rBV2	4371	9238	1.27%	0.207%
7	4.658	1007	1032	1063	rBV4	72886	274350	37.76%	6.136%
8	5.080	1145	1163	1188	rBV2	78882	180612	24.86%	4.039%
9	5.739	1346	1368	1389	rBV2	152297	395199	54.39%	8.838%
10	6.260	1516	1530	1547	rBV	127087	246631	33.94%	5.516%
11	6.552	1607	1621	1641	rBV	390768	726645	100.00%	16.251%
12	6.700	1653	1667	1689	rVB	112668	214420	29.51%	4.795%
13	7.575	1925	1939	1951	rBV2	51793	89320	12.29%	1.998%
14	7.906	2029	2042	2059	rBV	204179	354242	48.75%	7.922%
15	8.186	2118	2129	2143	rBV2	34251	57427	7.90%	1.284%
16	8.559	2232	2245	2258	rBV2	102944	172568	23.75%	3.859%
17	8.642	2258	2271	2295	rBV	285748	538134	74.06%	12.035%
18	9.420	2499	2513	2533	rBV	169823	286885	39.48%	6.416%
19	10.755	2916	2928	2945	rBV2	79171	128040	17.62%	2.864%
20	11.809	3244	3256	3269	rBV	152265	239988	33.03%	5.367%
21	12.189	3358	3374	3389	rBV	158876	254151	34.98%	5.684%




Sum of corrected areas: 4471406

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011421\
Data File : VU042051.D
Acq On : 14 Jan 2021 23:13
Operator : SY/MD
Sample : M1065-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXP1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

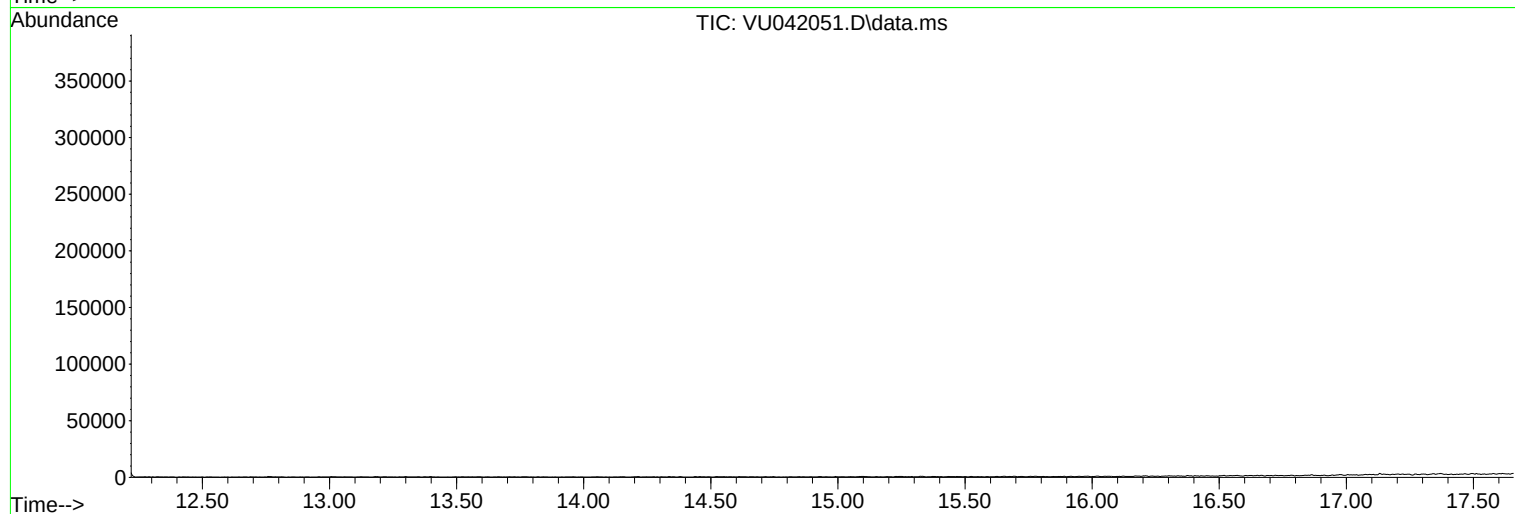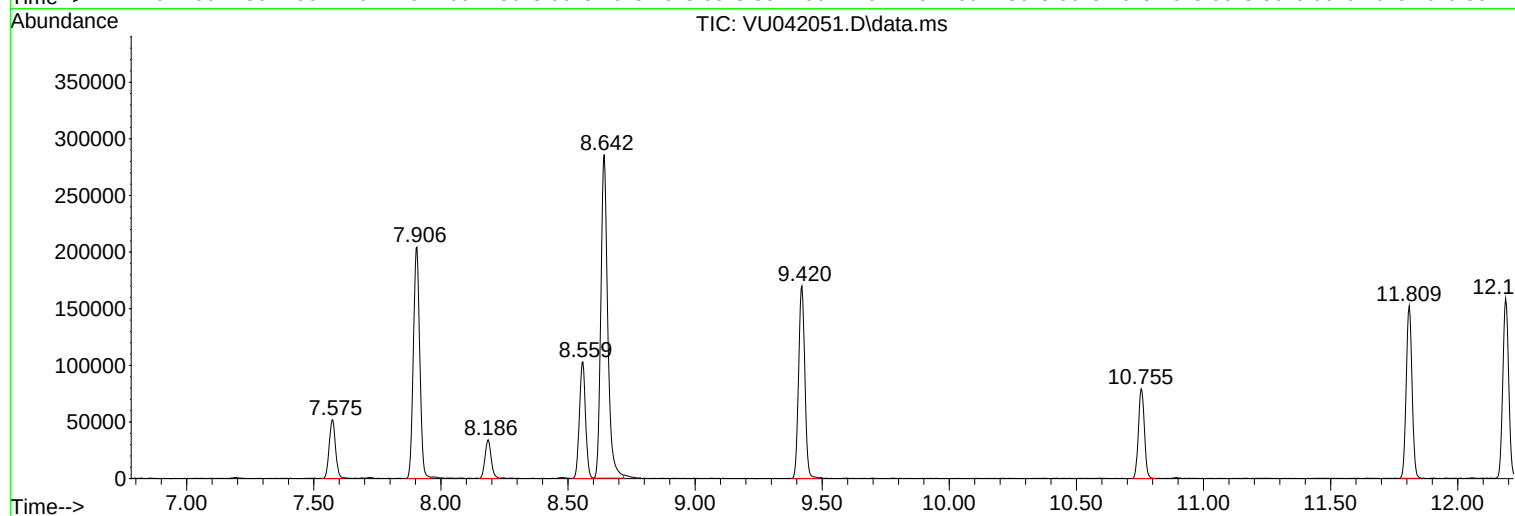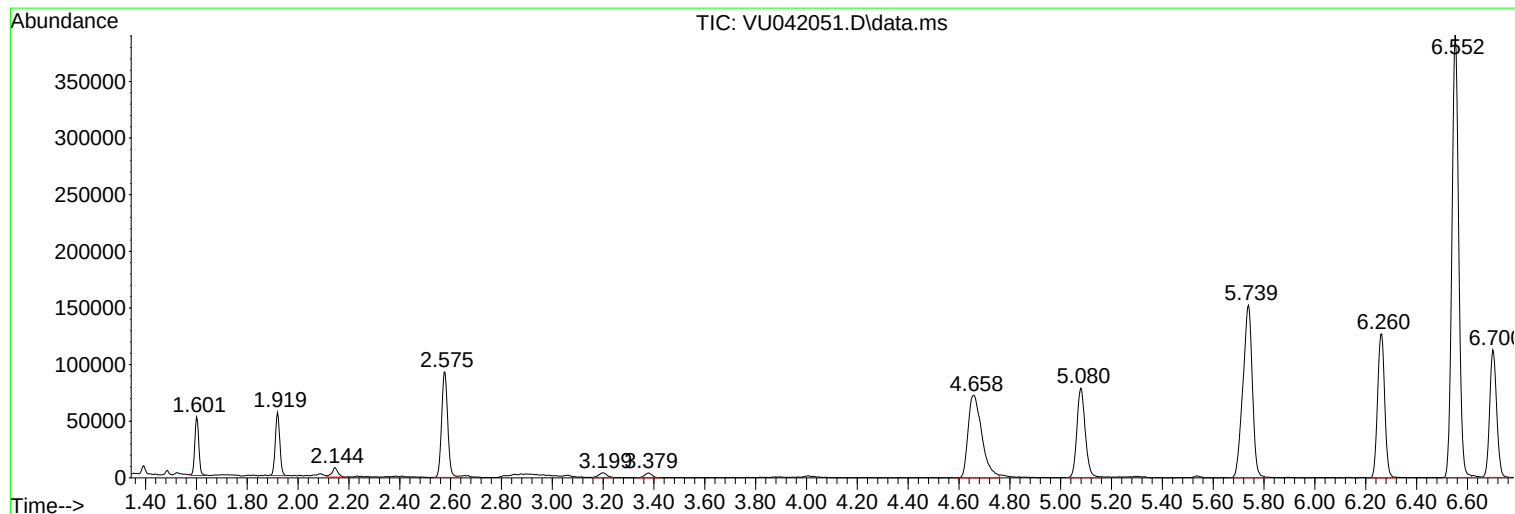

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011421\
Data File : VU042051.D
Acq On : 14 Jan 2021 23:13
Operator : SY/MD
Sample : M1065-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXP1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011421\
Data File : VU042051.D
Acq On : 14 Jan 2021 23:13
Operator : SY/MD
Sample : M1065-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXP1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
