


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011421\
 Data File : VU042021.D
 Acq On : 14 Jan 2021 09:33
 Operator : SY/MD
 Sample : BFB36
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB36

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Jan 16 01:05:16 2021

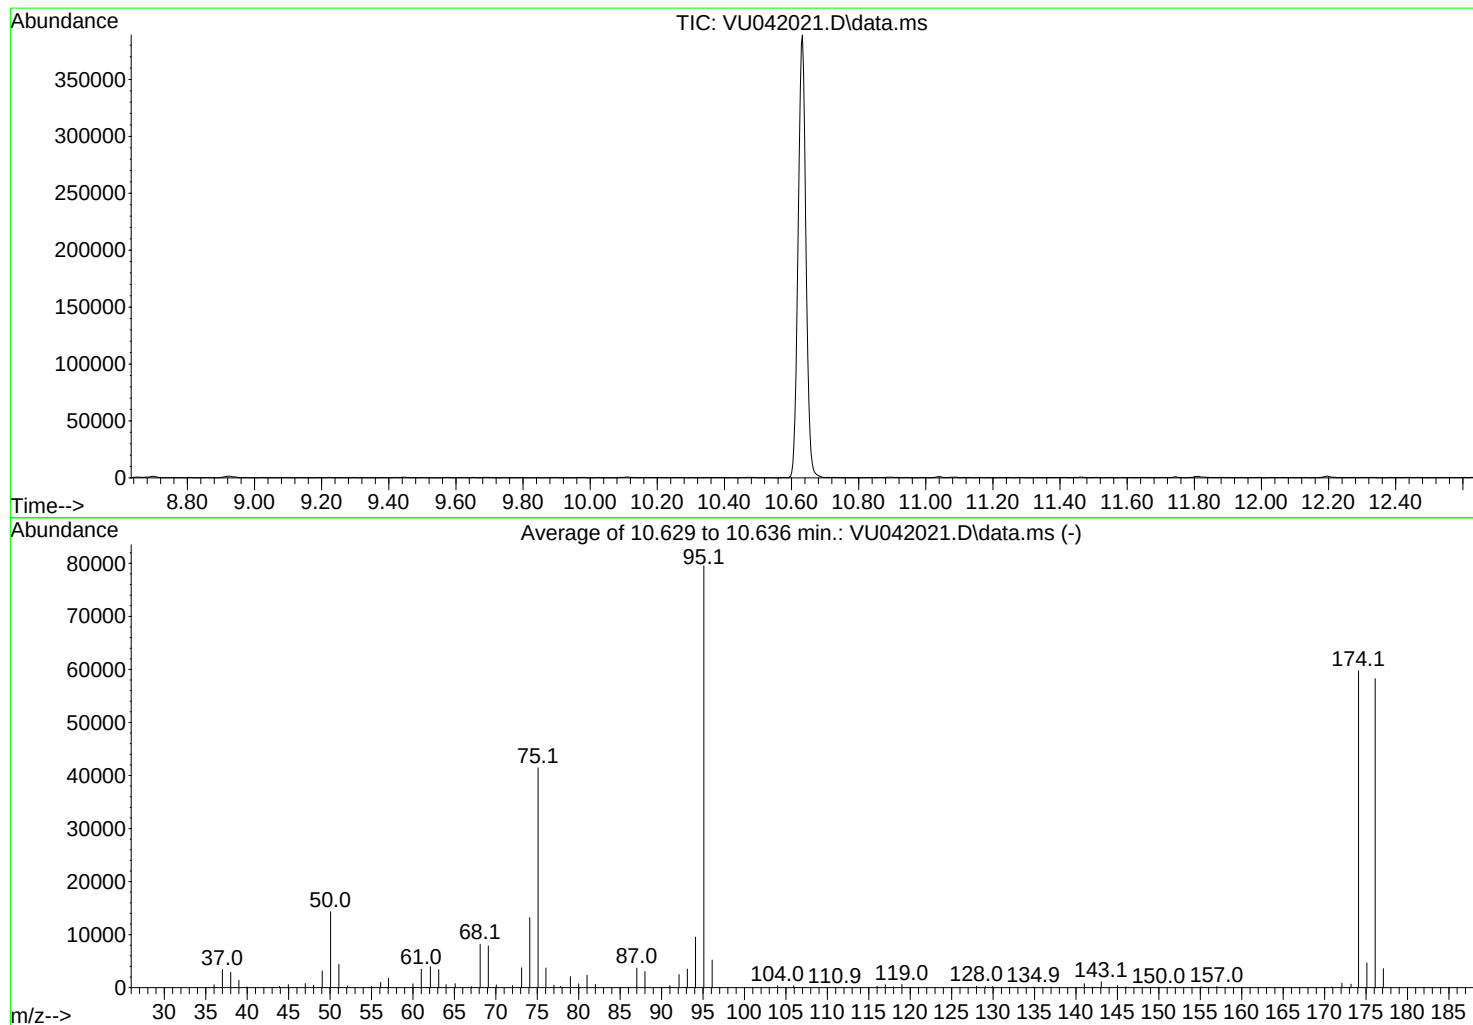

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	14332	PASS
75	95	30	80	52.1	41464	PASS
95	95	100	100	100.0	79528	PASS
96	95	5	9	6.5	5209	PASS
173	174	0.00	2	1.1	659	PASS
174	95	50	120	75.1	59723	PASS
175	174	5	9	7.8	4675	PASS
176	174	95	101	97.5	58251	PASS
177	176	5	9	6.2	3584	PASS

m/z	Abundance
43.90	190.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
36.00	593.0
37.00	3438.0
38.00	3050.0
39.00	1385.0
39.90	107.0
44.00	452.0
45.00	581.0
47.00	991.0
48.00	461.0
49.00	3262.0
50.10	14781.0
51.10	4760.0
52.10	292.0
55.00	191.0
56.10	921.0
57.00	1796.0
60.00	789.0
61.00	3523.0
62.10	4127.0
63.10	3420.0
64.00	649.0
65.10	756.0
67.00	200.0
68.10	8423.0
69.10	7904.0
70.10	548.0
72.00	453.0
73.10	3735.0
74.10	13427.0
75.10	41808.0
76.10	3950.0
77.00	498.0
77.80	217.0
79.00	2060.0
80.00	769.0
81.00	2312.0
82.00	569.0
85.90	135.0
87.00	3708.0
88.00	3279.0
91.00	398.0
92.10	2451.0
93.10	3413.0
94.10	9832.0
95.10	80616.0
96.10	5486.0
104.00	432.0
105.90	299.0
116.00	292.0
117.00	568.0
117.90	216.0
119.00	640.0
128.00	261.0
129.10	235.0
130.00	237.0
134.90	117.0
137.00	122.0
141.00	735.0
142.00	101.0
143.10	1047.0
145.00	412.0
146.10	182.0
148.00	127.0
155.10	251.0
157.00	211.0
170.90	173.0
172.10	862.0
173.20	938.0
174.10	59640.0
175.10	4644.0
176.10	58568.0
177.10	3630.0
178.00	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
36.00	556.0
37.00	3540.0
38.00	2986.0
39.00	1477.0
40.00	111.0
44.00	392.0
45.00	590.0
47.00	792.0
48.00	465.0
49.00	3274.0
50.10	14833.0
51.10	4550.0
52.10	315.0
55.00	221.0
56.10	1019.0
57.10	1784.0
60.00	783.0
61.00	3574.0
62.10	4096.0
63.10	3579.0
64.00	624.0
65.10	783.0
67.00	191.0
68.10	8477.0
69.10	8247.0
70.00	511.0
72.00	421.0
73.10	3798.0
74.10	13621.0
75.10	42912.0
76.10	3808.0
77.00	498.0
77.80	214.0
79.00	2126.0
80.00	746.0
81.00	2419.0
82.00	625.0
86.00	106.0
87.00	3832.0
88.00	3100.0
91.00	436.0
92.10	2581.0
93.10	3675.0
94.10	9870.0
95.10	82104.0
96.10	5380.0
104.00	341.0
105.90	339.0
110.90	121.0
115.10	104.0
116.00	290.0
117.00	569.0
118.00	167.0
119.00	635.0
128.00	269.0
129.10	173.0
130.00	204.0
134.90	118.0
137.00	127.0
141.00	786.0
142.10	156.0
143.00	1158.0
144.10	123.0
145.00	389.0
146.10	153.0
148.10	128.0
155.10	197.0
157.00	261.0
170.90	173.0
172.10	885.0
173.20	1039.0
174.10	61552.0
175.10	4833.0
176.10	60016.0
177.10	3667.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
36.00	521.0
37.00	3258.0
38.00	2624.0
39.00	1298.0
40.00	117.0
43.90	363.0
44.90	519.0
47.10	575.0
48.00	414.0
49.10	2989.0
50.00	13381.0
51.00	3887.0
52.10	307.0
55.00	208.0
56.10	1033.0
57.10	1683.0
60.00	651.0
61.00	3388.0
62.10	3653.0
63.10	3218.0
64.00	484.0
65.10	717.0
67.10	196.0
68.10	7597.0
69.10	7448.0
70.00	471.0
72.00	356.0
73.10	3685.0
74.10	12565.0
75.10	39672.0
76.00	3347.0
77.00	495.0
77.80	203.0
79.00	2039.0
80.00	660.0
81.00	2315.0
82.00	604.0
87.00	3502.0
88.00	2759.0
91.00	372.0
92.10	2411.0
93.10	3436.0
94.10	8930.0
95.10	75864.0
96.10	4761.0
97.10	108.0
104.00	276.0
106.00	341.0
115.00	102.0
116.00	239.0
117.00	536.0
118.00	161.0
119.00	502.0
128.00	251.0
129.10	108.0
129.90	188.0
134.90	117.0
137.00	100.0
141.00	757.0
142.10	154.0
143.00	1163.0
145.00	351.0
146.00	113.0
150.00	108.0
155.00	134.0
157.00	193.0
170.90	106.0
172.10	832.0
174.10	57976.0
175.10	4547.0
176.10	56168.0
177.10	3456.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36