




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011425\
Data File : VU062734.D
Acq On : 14 Jan 2025 11:20
Operator : MD/SY
Sample : Q1058-15
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH8Y4

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

Quant Time: Jan 15 00:32:42 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 15 00:31:11 2025
Response via : Initial Calibration

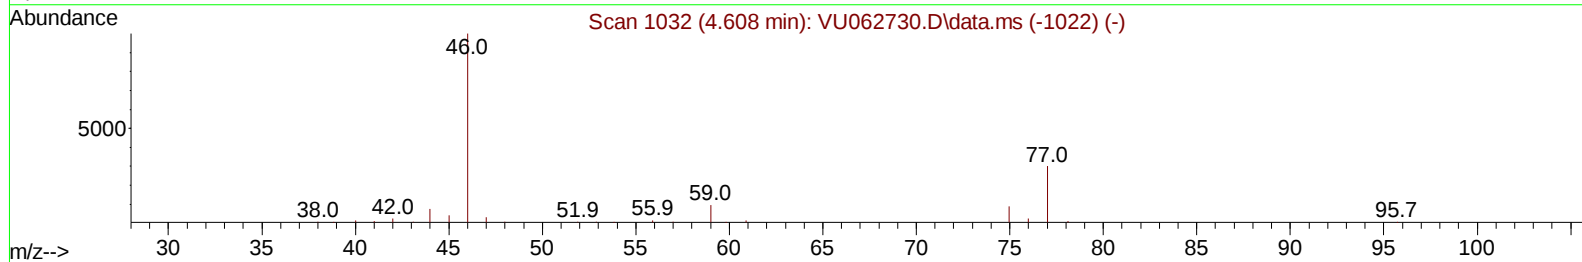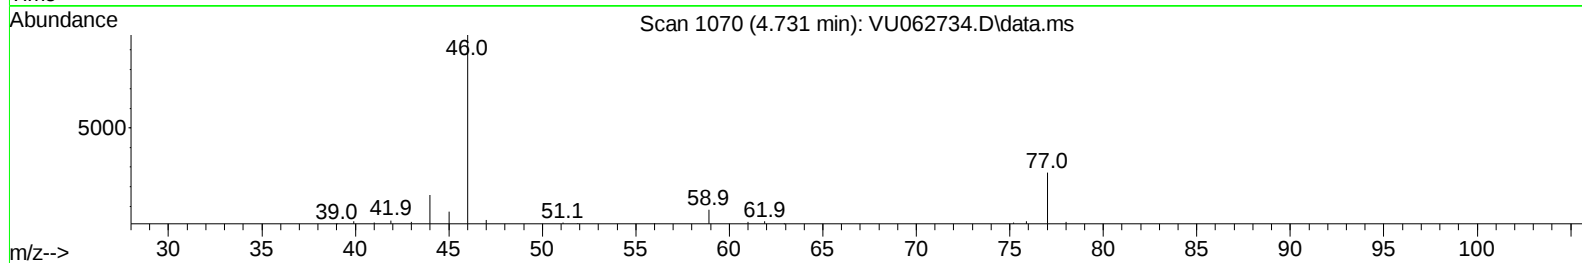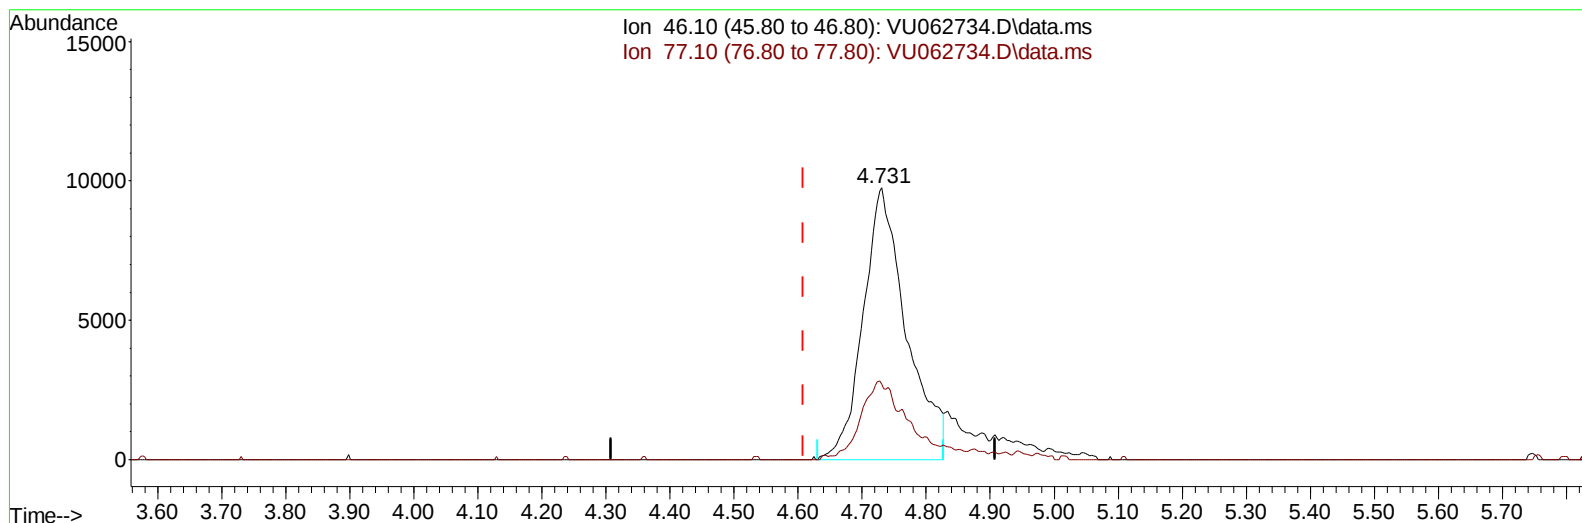

TIC: VU062734.D\data.ms

(20) 2-Butanone-d5 (S)

4.731min (+ 0.122) 43.62 ug/L

response 45647

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	30.90	19.76#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011425\
Data File : VU062734.D
Acq On : 14 Jan 2025 11:20
Operator : MD/SY
Sample : Q1058-15
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH8Y4

Manual IntegrationsAPPROVED

Quant Time: Jan 15 00:32:42 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 15 00:31:11 2025
Response via : Initial Calibration

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

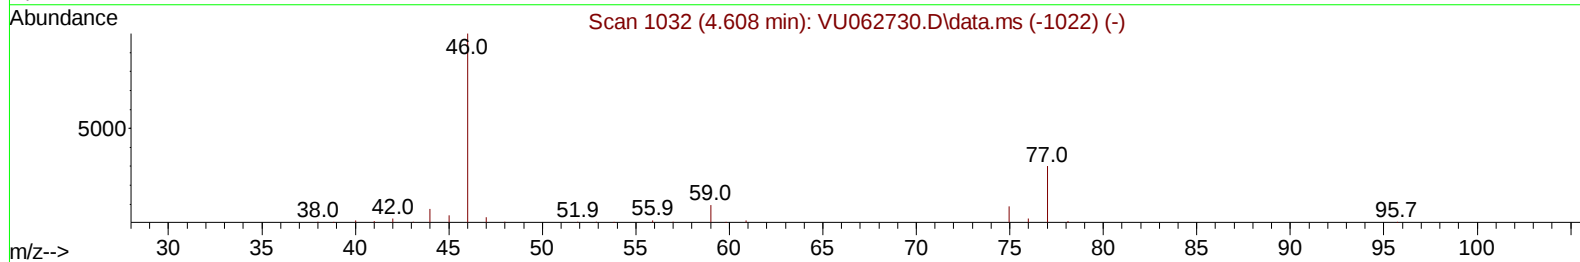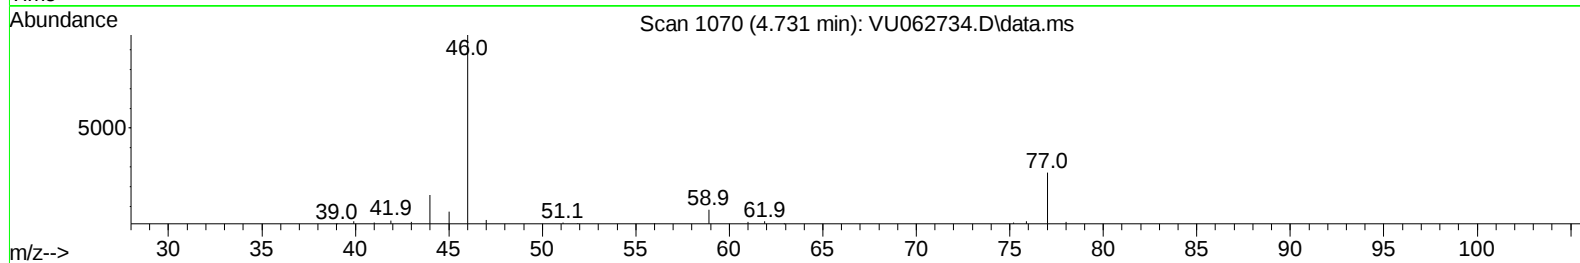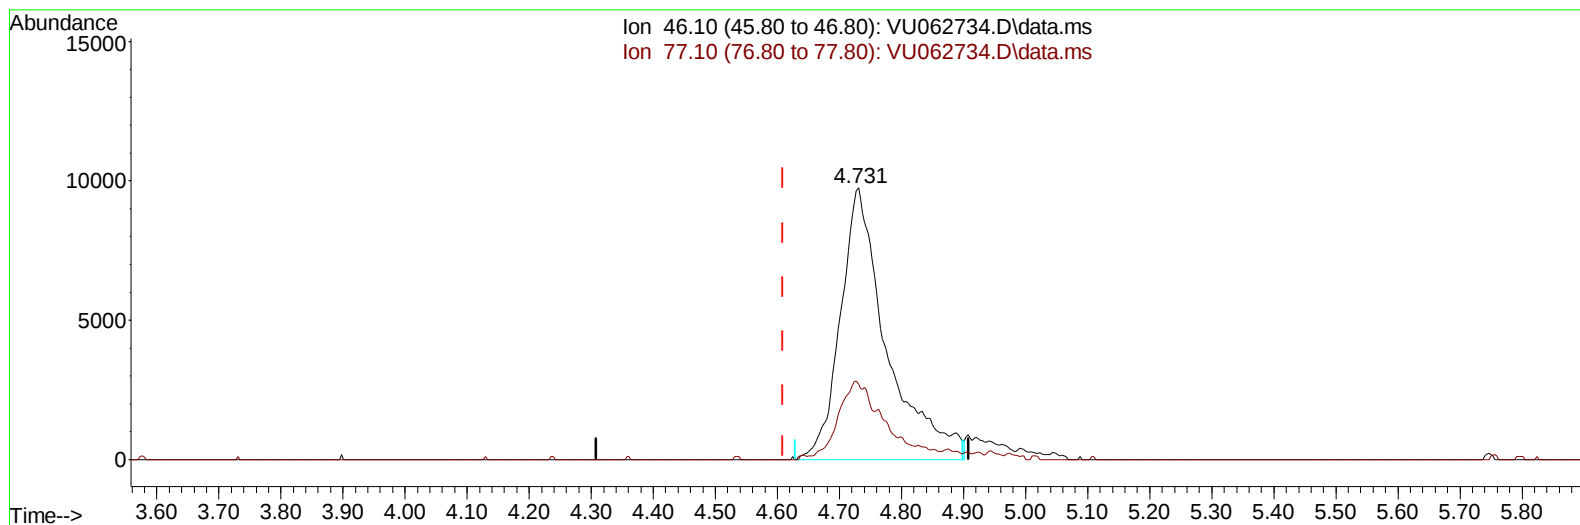

TIC: VU062734.D\data.ms

(20) 2-Butanone-d5 (S)

4.731min (+ 0.122) 48.26 ug/L m

response 50503

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	30.90	17.86#
0.00	0.00	0.00
0.00	0.00	0.00


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011425\
Data File : VU062734.D
Acq On : 14 Jan 2025 11:20
Operator : MD/SY
Sample : Q1058-15
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH8Y4

Manual IntegrationsAPPROVED

Quant Time: Jan 15 00:32:42 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 15 00:31:11 2025
Response via : Initial Calibration

Reviewed By :John Carlone 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

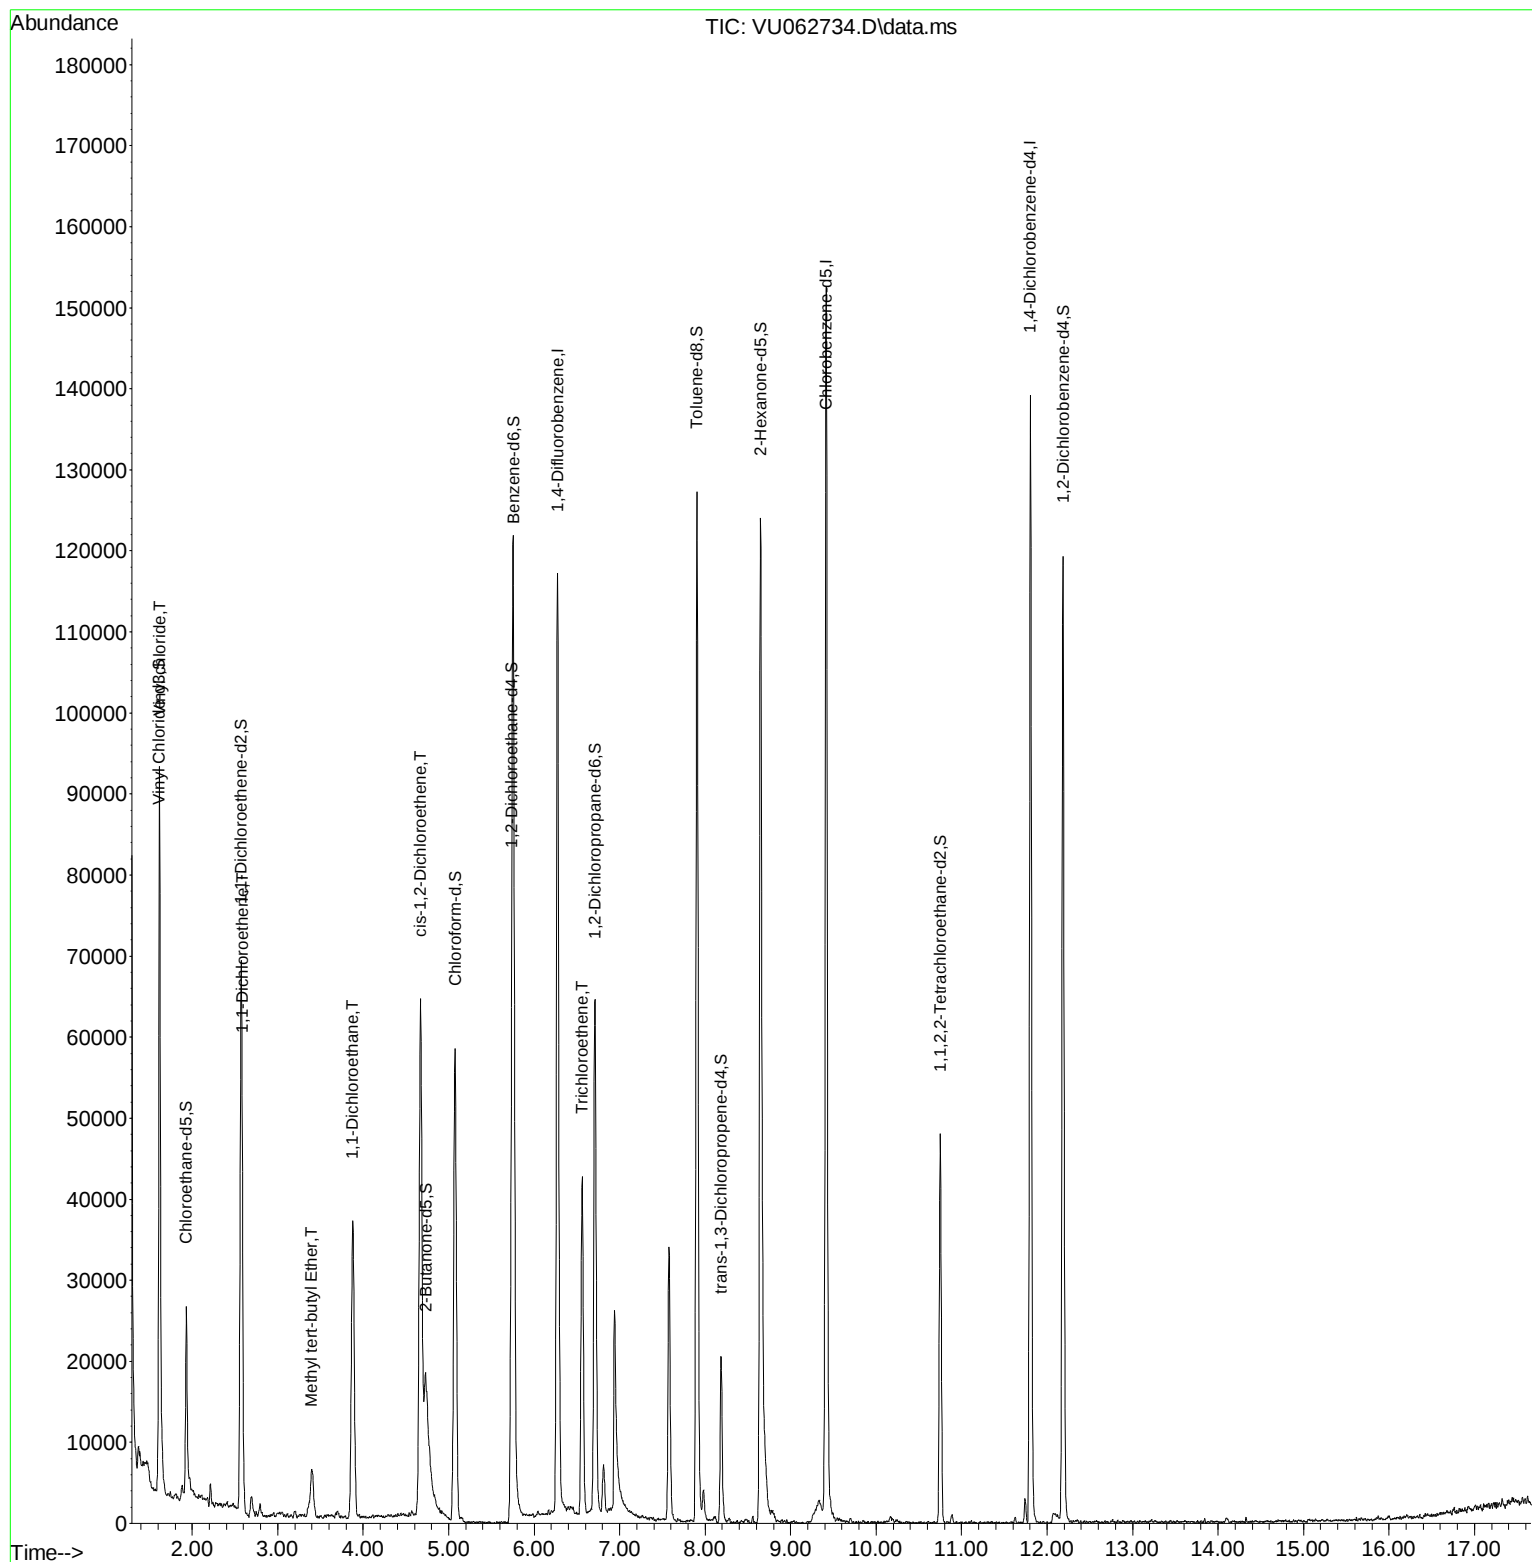

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011425\
 Data File : VU062734.D
 Acq On : 14 Jan 2025 11:20
 Operator : MD/SY
 Sample : Q1058-15
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH8Y4

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 01/15/2025
 Supervised By : Mahesh Dadoda 01/15/2025

Quant Time: Jan 15 00:32:42 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 15 00:31:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.274	114	92449	5.000	ug/L	0.03
28) Chlorobenzene-d5	9.415	117	83251	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	38723	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.612	65	17579	3.433	ug/L	0.02
Spiked Amount 5.000	Range 40	- 130	Recovery	=	68.600%	
7) Chloroethane-d5	1.930	69	15889	3.858	ug/L	0.03
Spiked Amount 5.000	Range 65	- 130	Recovery	=	77.200%	
11) 1,1-Dichloroethene-d2	2.570	65	9716	3.663	ug/L	0.01
Spiked Amount 5.000	Range 60	- 125	Recovery	=	73.200%	
20) 2-Butanone-d5	4.731	46	50503m	48.260	ug/L	0.12
Spiked Amount 50.000	Range 40	- 130	Recovery	=	96.520%	
24) Chloroform-d	5.075	84	57437	4.559	ug/L	0.03
Spiked Amount 5.000	Range 70	- 125	Recovery	=	91.200%	
26) 1,2-Dichloroethane-d4	5.737	65	32922	4.818	ug/L	0.05
Spiked Amount 5.000	Range 70	- 130	Recovery	=	96.400%	
32) Benzene-d6	5.756	84	95629	4.699	ug/L	0.04
Spiked Amount 5.000	Range 70	- 125	Recovery	=	94.000%	
36) 1,2-Dichloropropane-d6	6.708	67	28267	5.010	ug/L	0.03
Spiked Amount 5.000	Range 60	- 140	Recovery	=	100.200%	
41) Toluene-d8	7.904	98	88616	4.470	ug/L	0.02
Spiked Amount 5.000	Range 70	- 130	Recovery	=	89.400%	
43) trans-1,3-Dichloroprop...	8.184	79	11989	4.263	ug/L	0.02
Spiked Amount 5.000	Range 55	- 130	Recovery	=	85.200%	
46) 2-Hexanone-d5	8.647	63	47495	53.693	ug/L	0.03
Spiked Amount 50.000	Range 45	- 130	Recovery	=	107.380%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84	22741	4.813	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	96.200%	
66) 1,2-Dichlorobenzene-d4	12.187	152	31768	4.931	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	98.600%	
Target Compounds						
5) Vinyl chloride	1.618	62	54330	8.164	ug/L	99
12) 1,1-Dichloroethene	2.583	96	10007	1.744	ug/L #	67
17) Methyl tert-butyl Ether	3.396	73	7113	0.451	ug/L #	86
19) 1,1-Dichloroethane	3.875	63	39859	3.626	ug/L	96
22) cis-1,2-Dichloroethene	4.669	96	31622	4.723	ug/L	96
34) Trichloroethene	6.560	95	13925	1.704	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed