
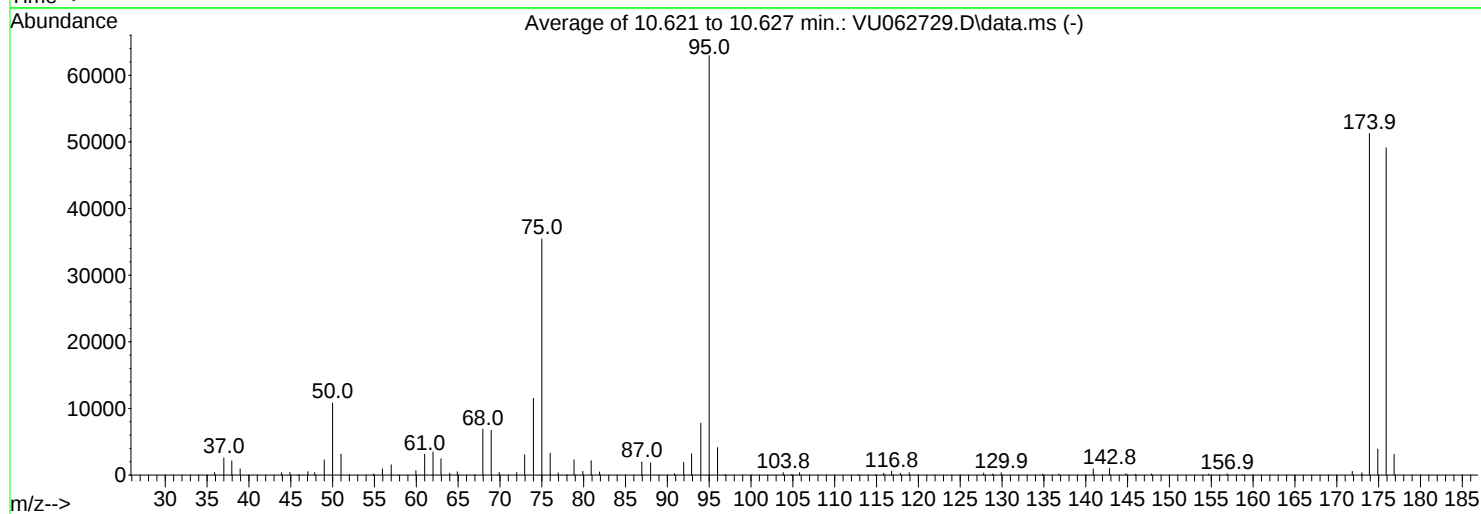


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011425\
Data File : VU062729.D
Acq On : 14 Jan 2025 08:07
Operator : MD/SY
Sample : BFB060
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB060

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jan 16 01:55:19 2025

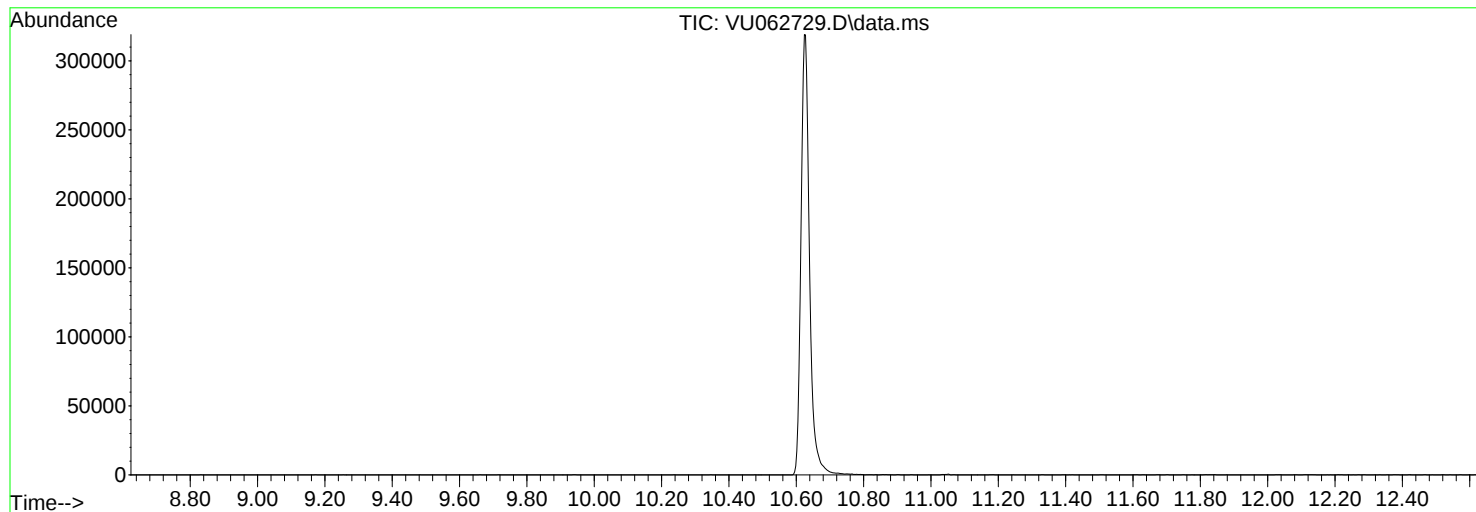

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	10817	PASS
75	95	30	80	56.3	35443	PASS
95	95	100	100	100.0	62936	PASS
96	95	5	9	6.6	4129	PASS
173	174	0.00	2	0.7	348	PASS
174	95	50	120	81.4	51251	PASS
175	174	5	9	7.6	3906	PASS
176	174	95	101	95.8	49123	PASS
177	176	5	9	6.4	3131	PASS

m/z Abundance

Instrument :
MSVOA_U
ClientSampleId :
BFB060

m/z	Abundance
35.90	385.0
37.00	2582.0
37.90	2067.0
39.00	873.0
43.90	292.0
44.90	426.0
47.10	566.0
47.90	340.0
49.00	2221.0
50.00	10266.0
51.00	3085.0
54.90	161.0
56.00	876.0
57.00	1520.0
60.00	637.0
61.00	3034.0
62.00	3385.0
62.90	2370.0
64.10	299.0
64.90	469.0
67.90	6631.0
68.90	6449.0
69.90	416.0
72.00	415.0
72.90	2983.0
74.00	10746.0
75.00	33680.0
76.00	3181.0
76.90	304.0
78.00	157.0
78.90	2169.0
79.90	512.0
80.90	1999.0
81.90	437.0
87.00	1814.0
88.00	1802.0
90.90	224.0
92.00	1809.0
92.90	3023.0
94.00	7310.0
95.00	59424.0
96.00	4046.0
103.90	369.0
105.80	333.0
115.90	214.0
116.80	498.0
117.90	271.0
118.90	347.0
127.80	289.0
128.90	135.0
129.90	366.0
134.90	144.0
136.80	125.0
140.90	763.0
142.80	896.0
144.80	231.0
146.00	100.0
147.80	146.0
154.70	136.0
156.90	195.0
158.70	101.0
171.80	573.0
173.00	502.0
173.90	47352.0
174.90	3582.0
175.90	45584.0
176.80	2913.0

Instrument :
MSVOA_U
ClientSampleId :
BFB060

m/z	Abundance
35.90	399.0
37.00	2665.0
38.00	2215.0
38.90	979.0
43.90	343.0
44.90	410.0
45.90	137.0
47.10	565.0
47.90	387.0
49.00	2299.0
50.00	11163.0
51.00	3256.0
54.90	178.0
56.00	939.0
57.00	1584.0
57.80	101.0
60.00	693.0
61.00	3208.0
62.00	3617.0
63.00	2527.0
64.00	291.0
64.90	520.0
67.90	7116.0
69.00	6939.0
69.90	401.0
72.00	430.0
72.90	3119.0
74.00	11711.0
75.00	36496.0
76.00	3423.0
77.00	327.0
78.90	2332.0
79.90	576.0
80.90	2202.0
81.90	467.0
86.90	2016.0
88.00	1814.0
90.90	226.0
91.90	1964.0
92.90	3315.0
94.00	8017.0
95.00	64792.0
96.00	4217.0
96.90	126.0
103.90	374.0
104.80	126.0
105.80	368.0
112.80	118.0
114.90	100.0
115.90	272.0
116.80	629.0
117.90	293.0
118.90	369.0
127.80	328.0
128.90	175.0
129.90	384.0
134.80	155.0
136.80	197.0
140.90	968.0
142.80	1004.0
144.80	224.0
146.00	123.0
147.90	182.0
154.70	157.0
156.90	214.0
171.80	591.0
173.00	542.0
173.90	52864.0
174.90	3998.0
175.90	50560.0
176.80	3204.0

Instrument :
MSVOA_U
ClientSampleId :
BFB060

m/z	Abundance
35.90	405.0
37.00	2451.0
38.00	2144.0
38.90	956.0
43.90	406.0
44.90	358.0
45.90	118.0
47.00	427.0
47.80	397.0
49.00	2325.0
50.00	11022.0
51.00	3136.0
52.00	112.0
54.90	178.0
55.90	970.0
57.00	1562.0
59.90	637.0
61.00	3155.0
62.00	3471.0
63.00	2479.0
63.90	259.0
64.90	500.0
67.00	123.0
68.00	6967.0
69.00	6794.0
69.90	374.0
72.00	371.0
73.00	3038.0
74.00	12109.0
75.00	36152.0
76.00	3284.0
77.00	355.0
78.80	2367.0
79.90	633.0
80.90	2287.0
81.90	502.0
86.90	2107.0
88.00	1845.0
90.80	218.0
91.90	1992.0
92.90	3216.0
94.00	8038.0
95.00	64592.0
96.00	4125.0
96.90	131.0
103.80	381.0
104.90	145.0
105.80	354.0
112.80	116.0
115.80	293.0
116.80	654.0
117.80	294.0
118.90	393.0
127.80	334.0
128.90	209.0
129.90	348.0
134.80	141.0
136.80	248.0
140.90	1057.0
142.90	1052.0
144.80	175.0
145.90	118.0
147.90	190.0
154.70	178.0
156.90	206.0
158.80	113.0
171.90	530.0
173.90	53536.0
174.90	4138.0
175.90	51224.0
176.90	3276.0

Instrument :
MSVOA_U
ClientSampleId :
BFB060