


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU011519\
 Data File : VU029170.D
 Acq On : 15 Jan 2019 08:45
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
 Title : SW846 8260
 Last Update : Sat Jan 12 01:33:59 2019

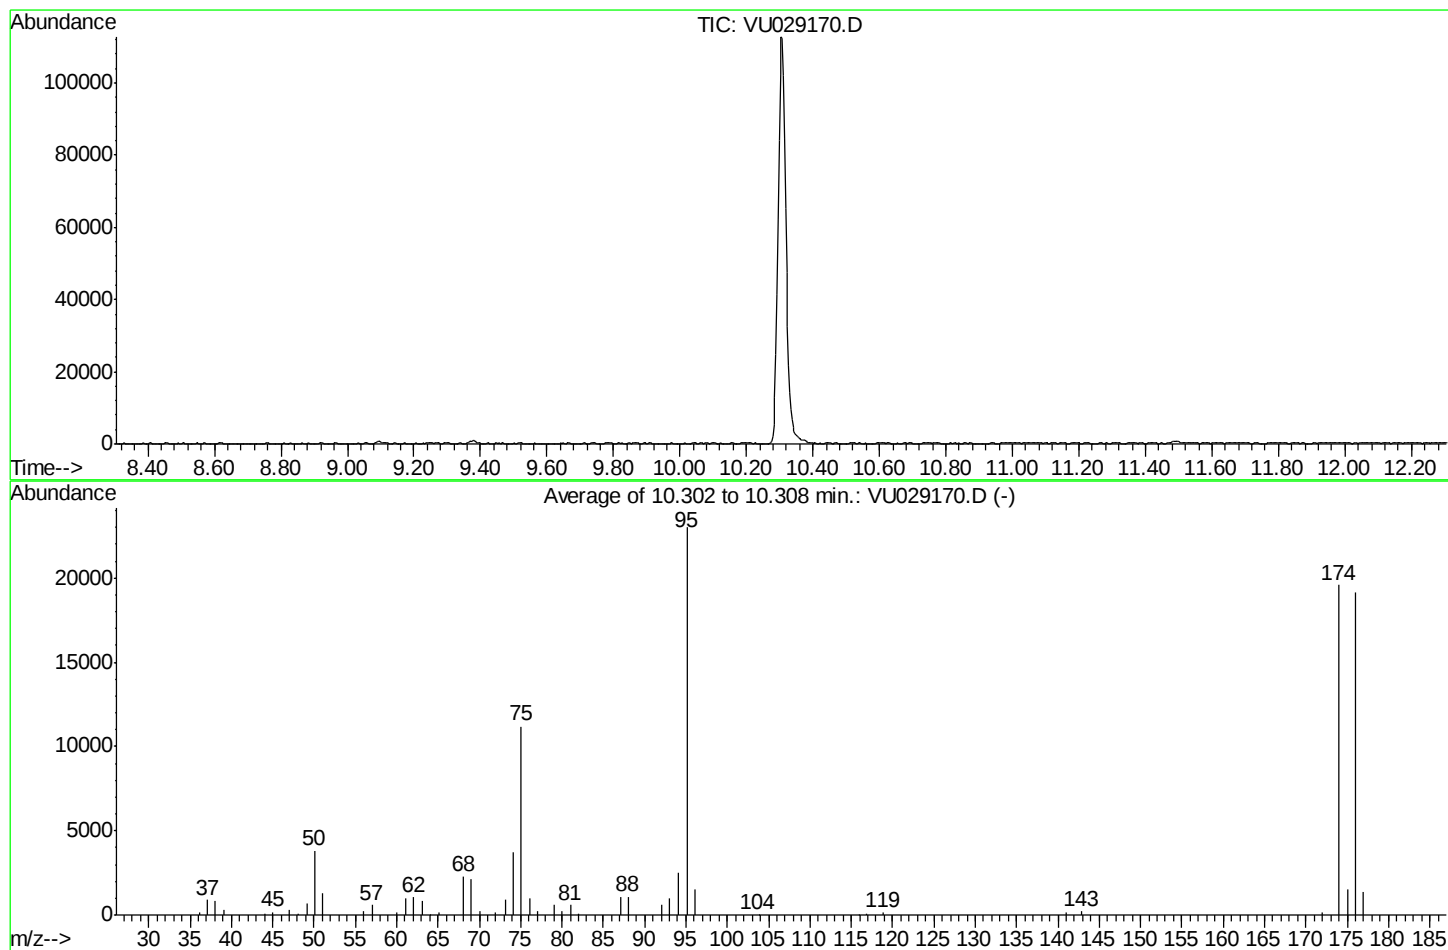

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	3800	PASS
75	95	30	60	48.6	11179	PASS
95	95	100	100	100.0	23005	PASS
96	95	5	9	6.8	1559	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.0	19562	PASS
175	174	5	9	7.6	1496	PASS
176	174	95	101	97.7	19114	PASS
177	176	5	9	7.2	1369	PASS