
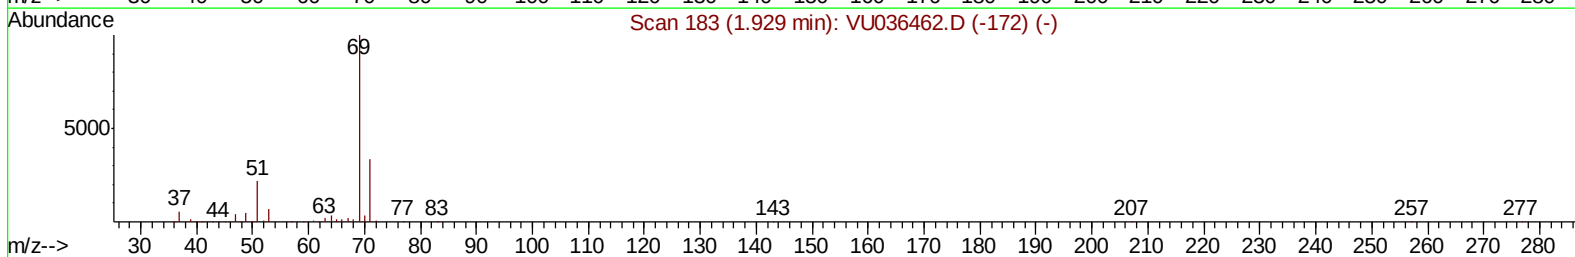
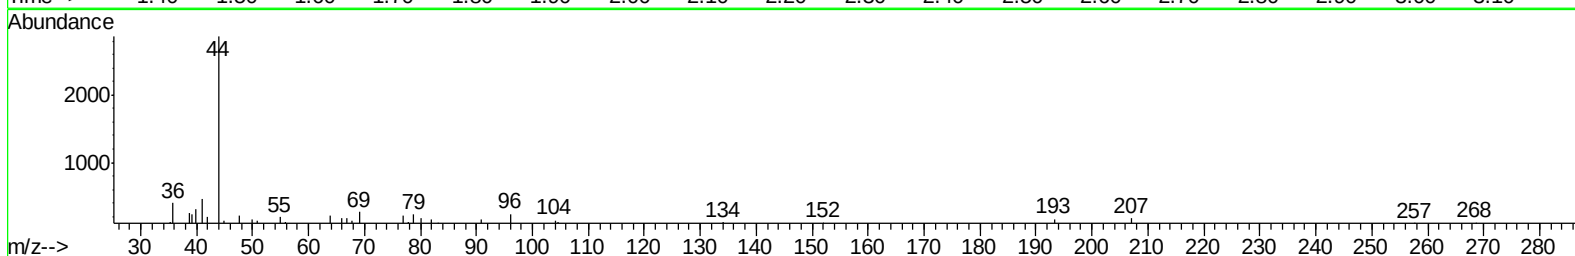


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU011520\
Data File : VU036473.D
Acq On : 15 Jan 2020 16:21
Operator : JC/MD
Sample : L1090-11
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 05:59:40 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 16 05:57:22 2020
Response via : Initial Calibration

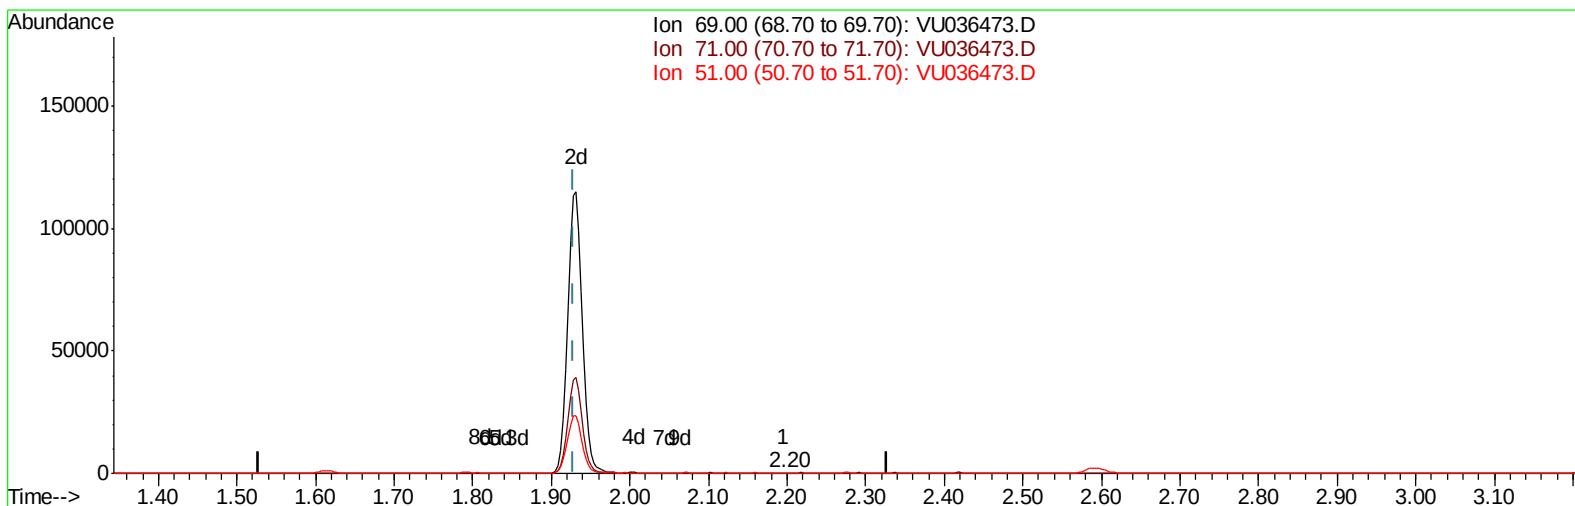

TIC: VU036473.D

(7) Chloroethane-d5 (S)

2.195min (+0.267) 0.07ug/L

response 180

Ion	Exp%	Act%
69.00	100	100
71.00	32.30	24.44
51.00	30.20	31.11
0.00	0.00	0.00