
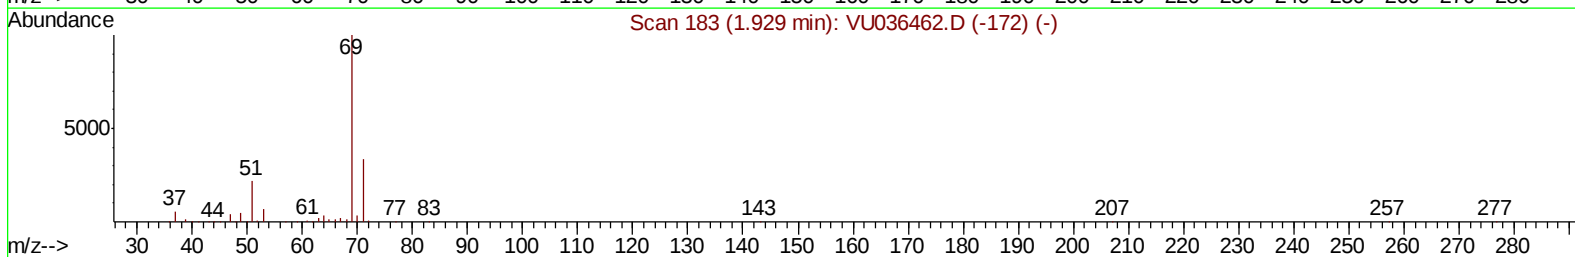
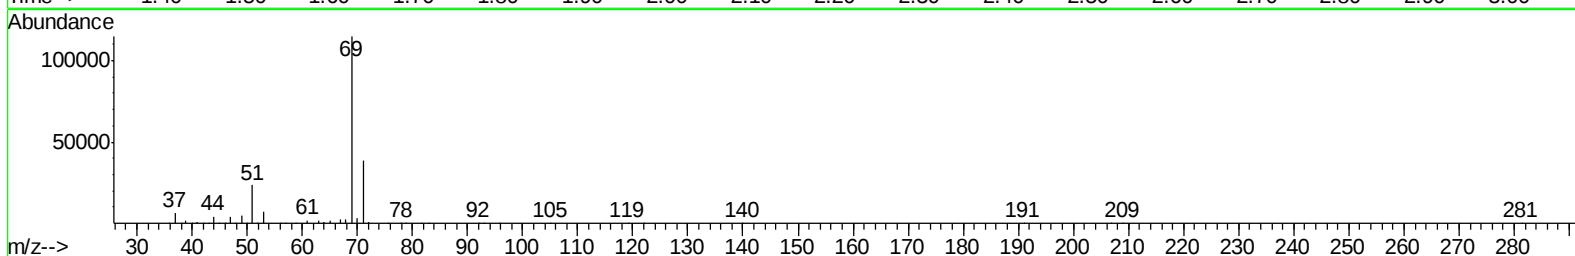


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU011520\
 Data File : VU036473.D
 Acq On : 15 Jan 2020 16:21
 Operator : JC/MD
 Sample : L1090-11
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 05:59:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 16 05:57:22 2020
 Response via : Initial Calibration

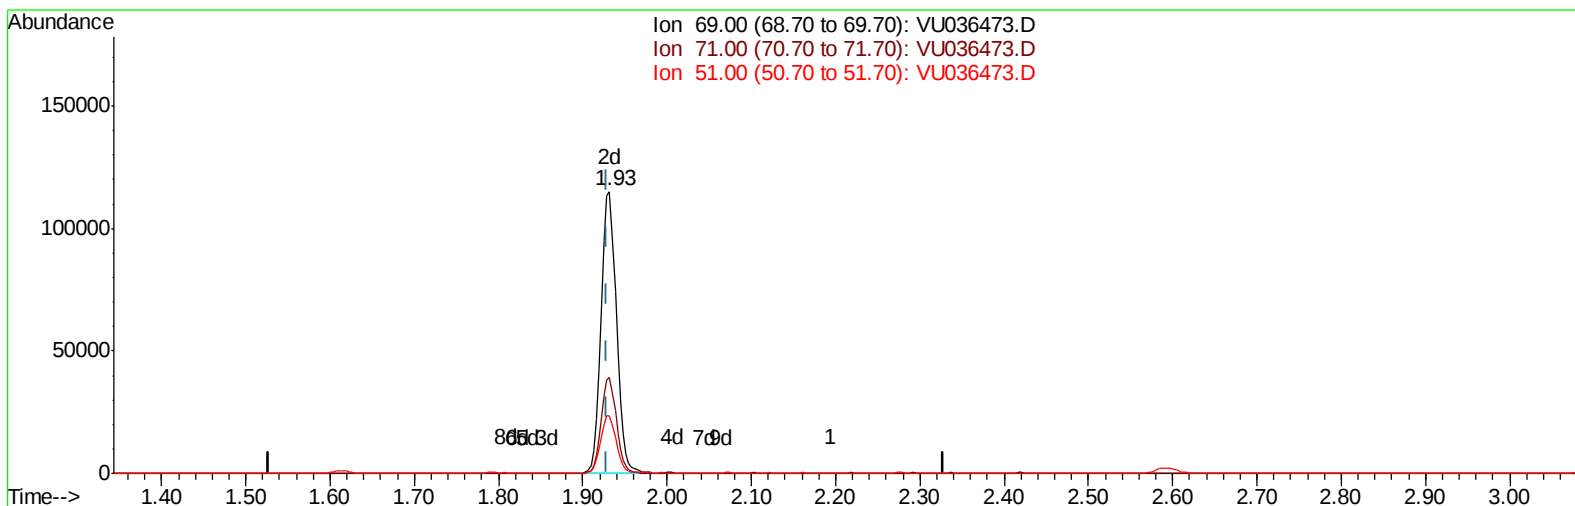

TIC: VU036473.D

(7) Chloroethane-d5 (S)

1.932min (+0.003) 55.51ug/L m

response 146789

Ion	Exp%	Act%
69.00	100	100
71.00	32.30	0.03#
51.00	30.20	0.04#
0.00	0.00	0.00