
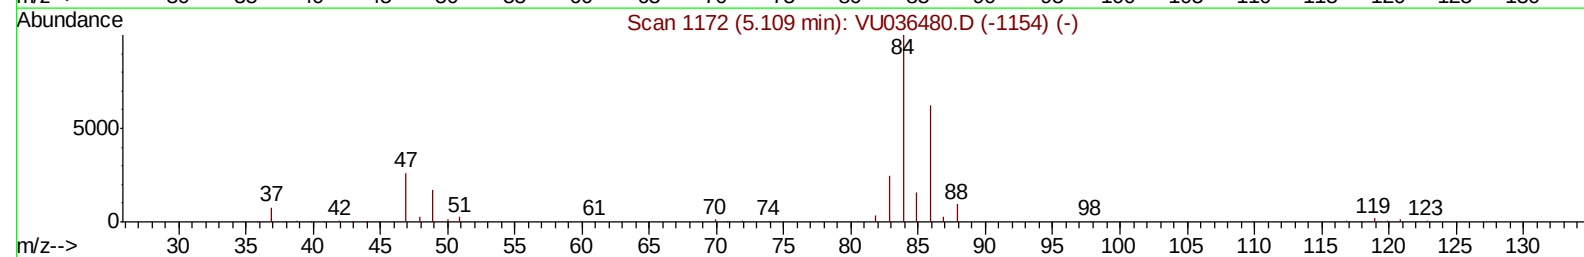
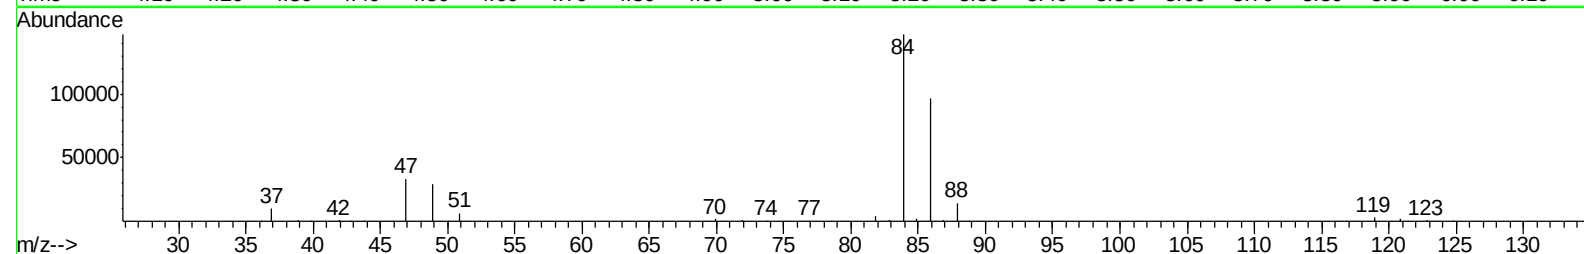


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU011520\
 Data File : VU036490.D
 Acq On : 16 Jan 2020 00:39
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 06:55:44 2020
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 16 06:52:15 2020
 Response via : Initial Calibration

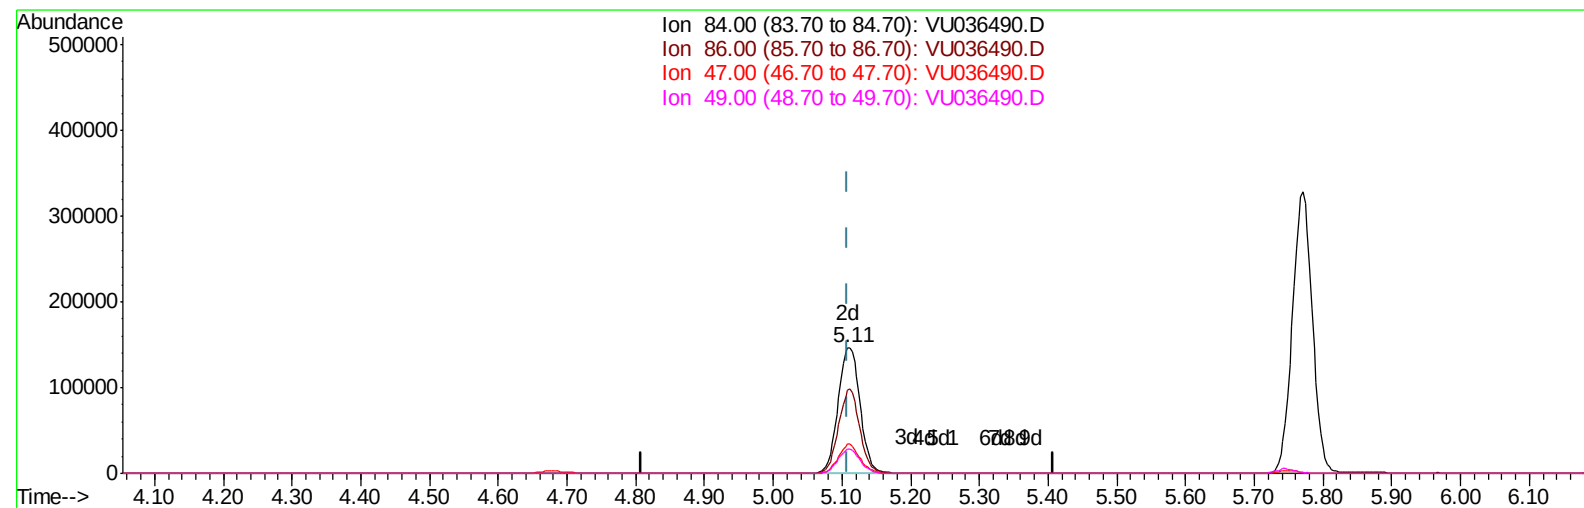

TIC: VU036490.D

(24) Chloroform-d (S)

5.108min (-0.000) 46.90ug/L m

response 325642

Ion	Exp%	Act%
84.00	100	100
86.00	62.80	0.04#
47.00	47.10	0.03#
49.00	28.40	0.02#