

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU011520\
Data File : VU036477.D
Acq On : 15 Jan 2020 18:15
Operator : JC/MD
Sample : L1139-04
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D50

Manual Integrations
APPROVED

apatel
1/16/2020 12:04:17 PM

Quant Time: Jan 16 06:00:04 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 16 05:57:22 2020
Response via : Initial Calibration

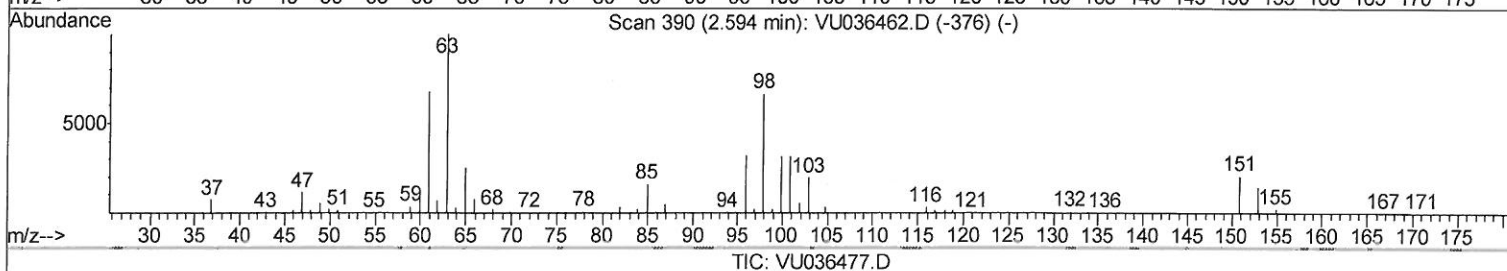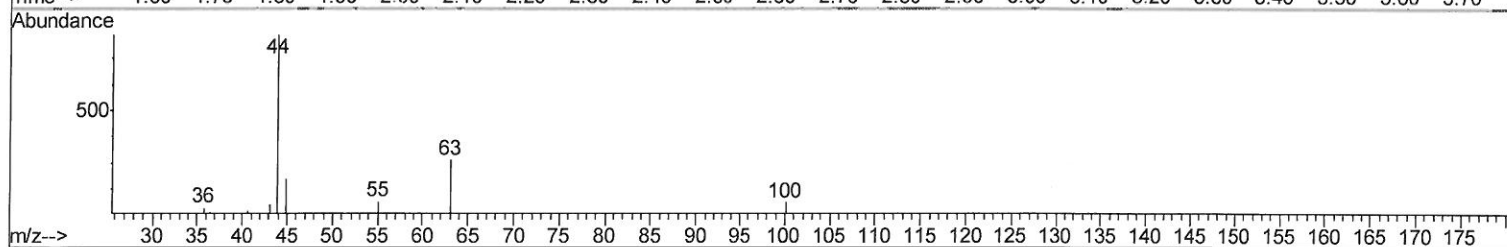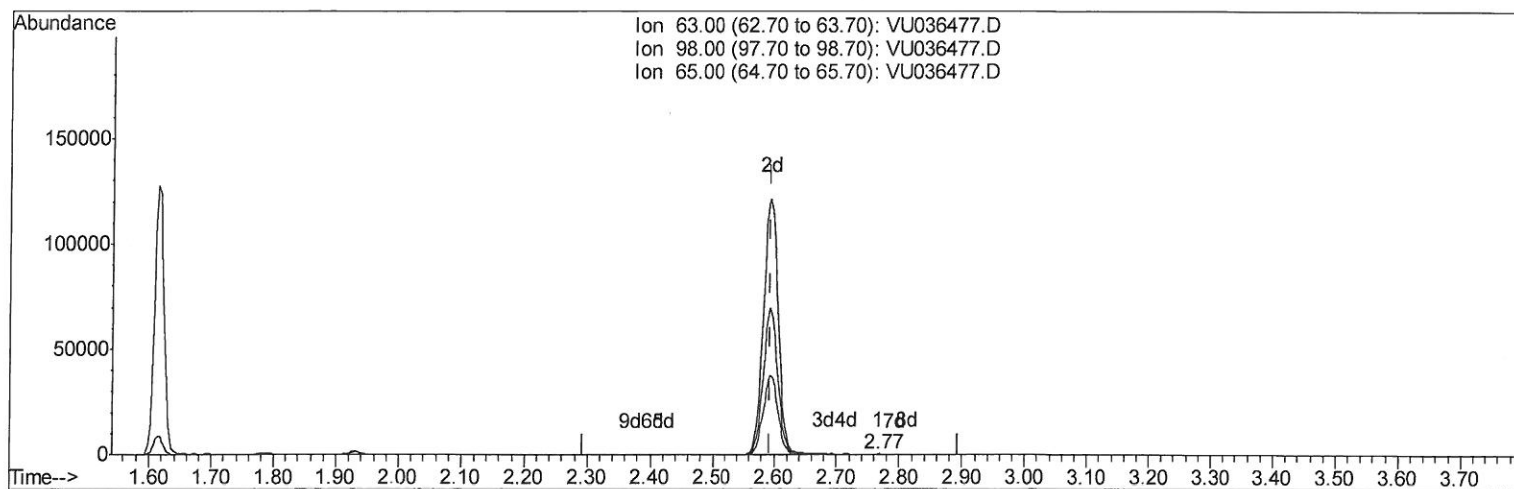

TIC: VU036477.D

(11) 1,1-Dichloroethene-d2 (S)

2.768min (+0.174) 0.06ug/L

response 312

Ion	Exp%	Act%
63.00	100	100
98.00	72.30	69.23
65.00	23.30	22.76
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU011520\
Data File : VU036477.D
Acq On : 15 Jan 2020 18:15
Operator : JC/MD
Sample : L1139-04
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D50

Manual Integrations
APPROVED

apatel
1/16/2020 12:04:17 PM

Quant Time: Jan 16 06:00:04 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 16 05:57:22 2020
Response via : Initial Calibration

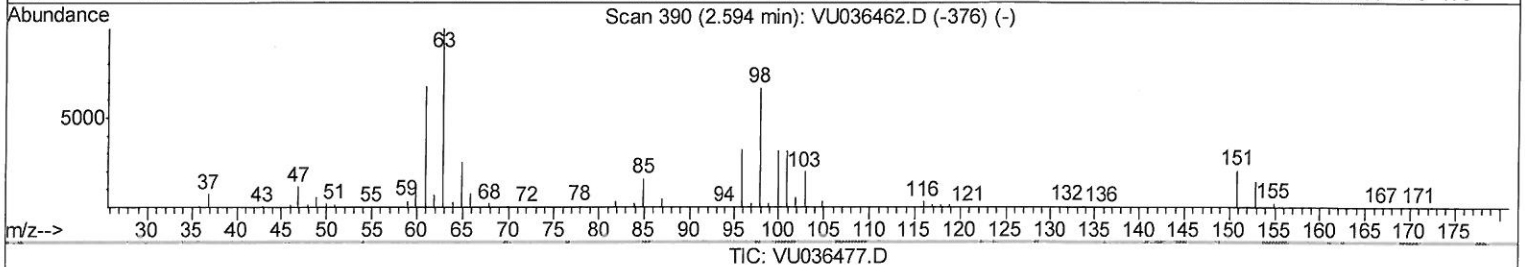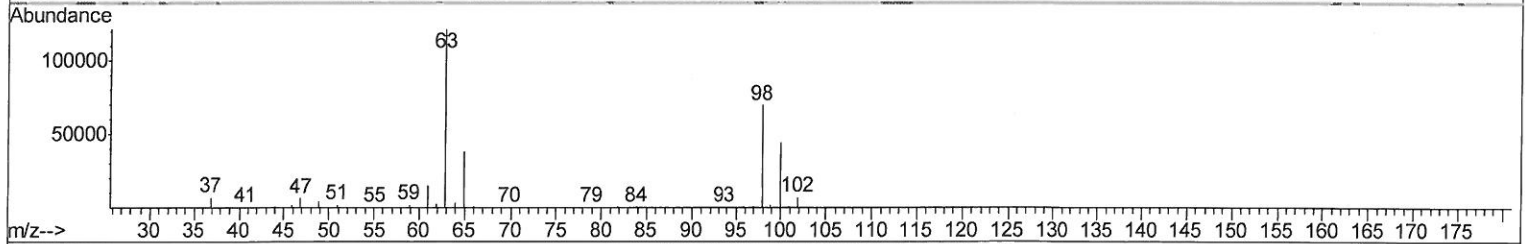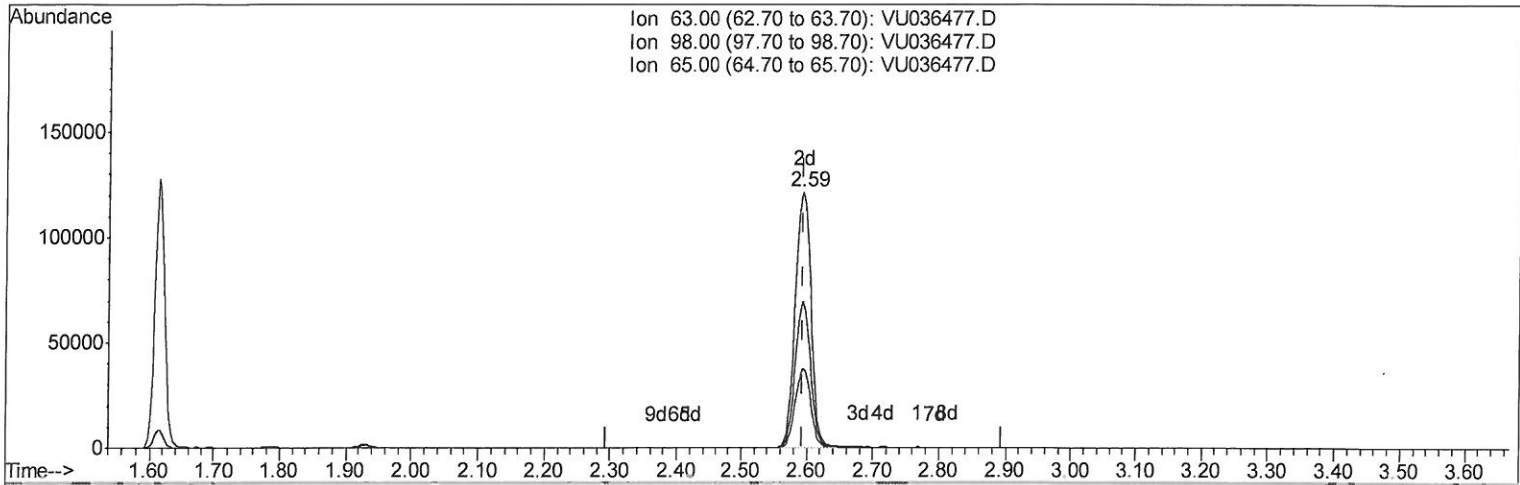

(11) 1,1-Dichloroethene-d2 (S)

2.594min (-0.000) 36.14ug/L m

response 203292

Ion	Exp%	Act%
63.00	100	100
98.00	72.30	0.11#
65.00	23.30	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU011520\
 Data File : VU036477.D
 Acq On : 15 Jan 2020 18:15
 Operator : JC/MD
 Sample : L1139-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D50

Manual Integrations
 APPROVED

apatel
 1/16/2020 12:04:17 PM

Quant Time: Jan 16 06:41:04 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 16 05:57:22 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	451802	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	424304	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	151859	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	135084	46.12	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.24%
7) Chloroethane-d5	1.93	69	123760	48.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.62%
11) 1,1-Dichloroethene-d2	2.59	63	203292m	36.14	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.28%
21) 2-Butanone-d5	4.68	46	254941	101.23	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.23%
24) Chloroform-d	5.11	84	287989	49.38	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.76%
26) 1,2-Dichloroethane-d4	5.75	65	200665	51.76	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.52%
32) Benzene-d6	5.77	84	557811	50.27	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.54%
36) 1,2-Dichloropropane-d6	6.73	67	187004	51.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.64%
41) Toluene-d8	7.93	98	521368	49.67	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.34%
43) trans-1,3-Dichloropropene-	8.21	79	93906	48.30	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.60%
47) 2-Hexanone-d5	8.67	63	183916	99.45	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.45%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	266959	49.18	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.36%
64) 1,2-Dichlorobenzene-d4	12.22	152	156478	52.31	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.62%

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
25) Chloroform	5.14	83	30463	5.168	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU011520\
Data File : VU036477.D
Acq On : 15 Jan 2020 18:15
Operator : JC/MD
Sample : L1139-04
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D50

Manual Integrations
APPROVED

apatel
1/16/2020 12:04:17 PM

Quant Time: Jan 16 06:41:04 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 16 05:57:22 2020
Response via : Initial Calibration

