

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU011520\
 Data File : VU036486.D
 Acq On : 15 Jan 2020 22:59
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK42

Manual Integrations
 APPROVED

apatel
 1/16/2020 12:05:46 PM

Quant Time: Jan 16 06:55:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 16 06:52:15 2020
 Response via : Initial Calibration

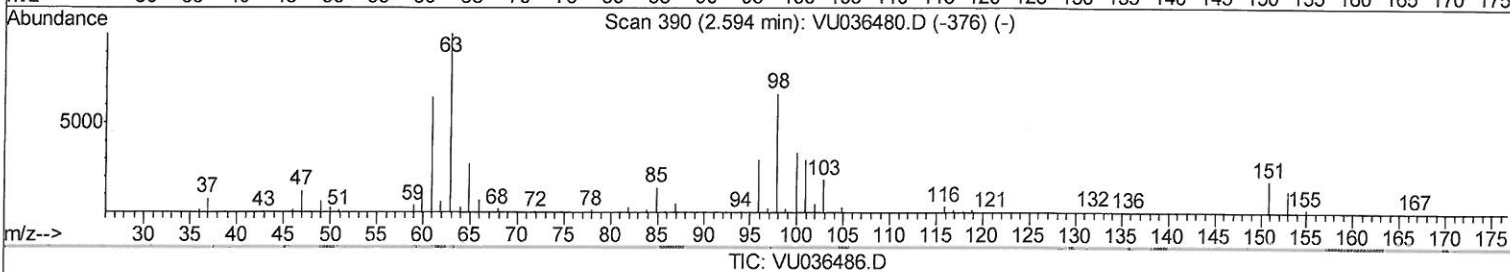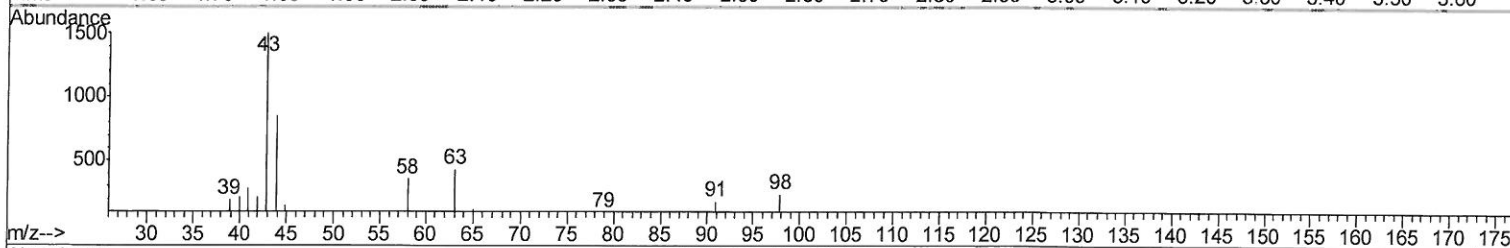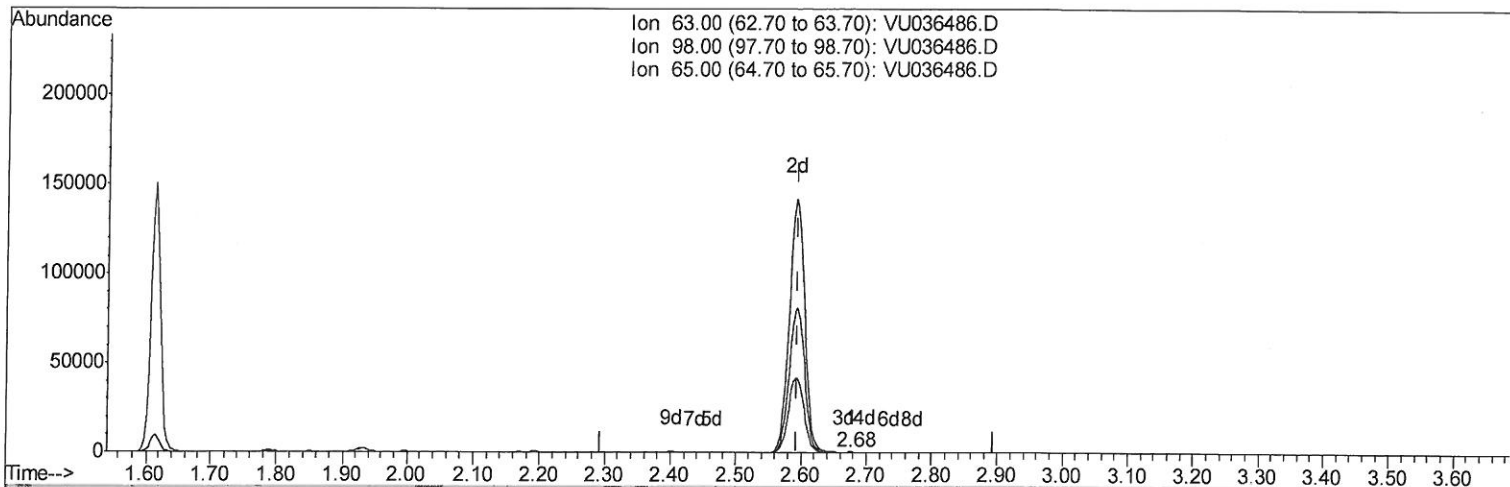

TIC: VU036486.D

(11) 1,1-Dichloroethene-d2 (S)

2.678min (+0.083) 0.04ug/L

response 254

Ion	Exp%	Act%
63.00	100	100
98.00	72.30	70.87
65.00	23.30	16.93
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU011520\
 Data File : VU036486.D
 Acq On : 15 Jan 2020 22:59
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
ClientSampleId :
 VIBLK42

Manual Integrations
APPROVED

apatel
 1/16/2020 12:05:46 PM

Quant Time: Jan 16 06:55:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 16 06:52:15 2020
 Response via : Initial Calibration

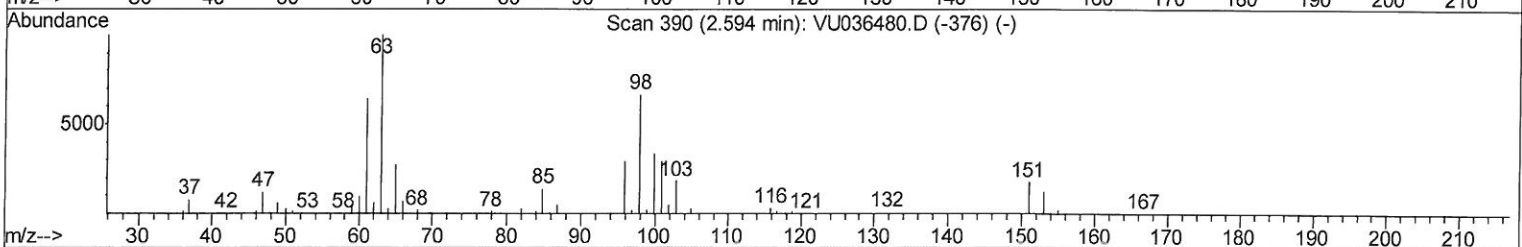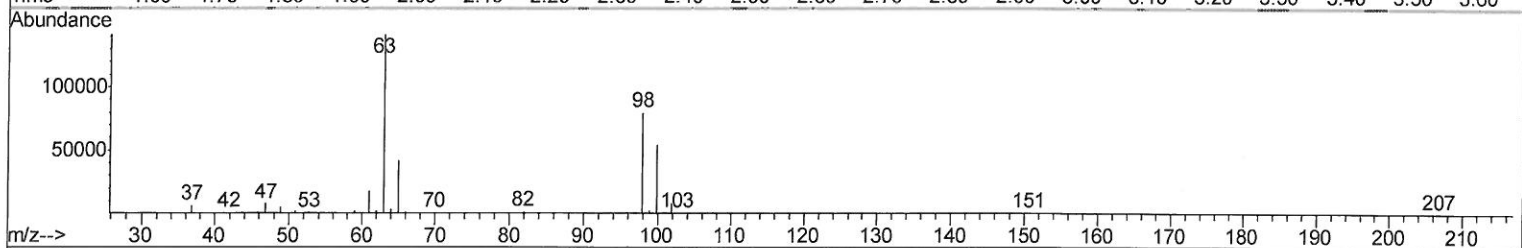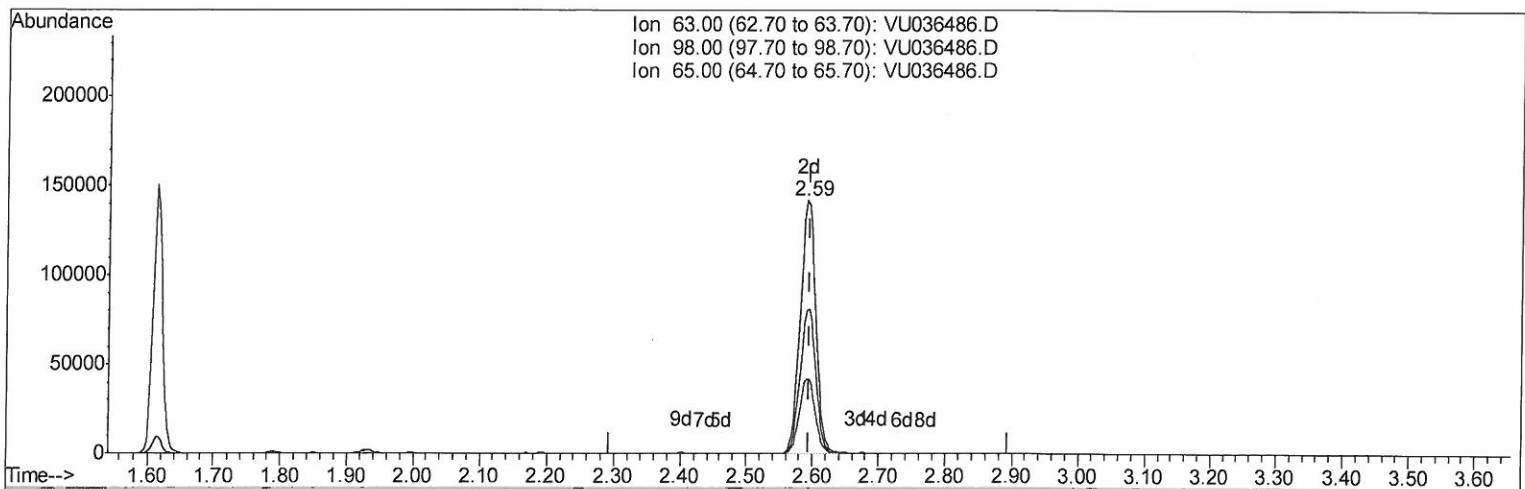

TIC: VU036486.D

(11) 1,1-Dichloroethene-d2 (S)

2.591min (-0.003) 34.38ug/L m

response 230388

Ion	Exp%	Act%
63.00	100	100
98.00	72.30	0.08#
65.00	23.30	0.02#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU011520\
 Data File : VU036486.D
 Acq On : 15 Jan 2020 22:59
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK42

Manual Integrations
 APPROVED

apatel
 1/16/2020 12:05:46 PM

Quant Time: Jan 16 07:44:33 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 16 06:52:15 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	538272	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	500455	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	236932	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	156065	44.72	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	89.44%		
7) Chloroethane-d5	1.93	69	145992	48.33	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	96.66%		
11) 1,1-Dichloroethene-d2	2.59	63	230388m	34.38	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	68.76%		
21) 2-Butanone-d5	4.68	46	298143	99.37	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	99.37%		
24) Chloroform-d	5.11	84	320796	46.17	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.34%		
26) 1,2-Dichloroethane-d4	5.74	65	223749	48.44	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.88%		
32) Benzene-d6	5.77	84	649061	49.59	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.18%		
36) 1,2-Dichloropropane-d6	6.73	67	217682	51.14	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	102.28%		
41) Toluene-d8	7.93	98	600393	48.50	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.00%		
43) trans-1,3-Dichloropropene-	8.21	79	109327	47.68	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	95.36%		
47) 2-Hexanone-d5	8.67	63	230867	105.84	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	105.84%		
57) 1,1,2,2-Tetrachloroethane-	10.78	84	318705	49.78	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	99.56%		
64) 1,2-Dichlorobenzene-d4	12.21	152	233587	50.05	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.10%		

Target Compounds

					Ovalue
13) Acetone	2.66	43	7172	2.209	ug/L 94
25) Chloroform	5.14	83	16852	2.400	ug/L 93
53) m,p-Xylene	9.72	106	7665	1.175	ug/L 70

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU011520\
Data File : VU036486.D
Acq On : 15 Jan 2020 22:59
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
VIBLK42

Manual Integrations
APPROVED

apatel
1/16/2020 12:05:46 PM

Quant Time: Jan 16 07:44:33 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 16 06:52:15 2020
Response via : Initial Calibration

