

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU011520\
 Data File : VU036482.D
 Acq On : 15 Jan 2020 21:19
 Operator : JC/MD
 Sample : L1118-12
 Misc : 5.01G/5.0mL/100uL/5.0mL/MSVOA_U/METHANOL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GASK3

Quant Time: Jan 16 07:02:29 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 16 06:52:15 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	899876	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	882414	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	394736	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	344112	58.98	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	117.96%
7) Chloroethane-d5	1.89	69	267098	52.89	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	105.78%
11) 1,1-Dichloroethene-d2	2.56	63	547091	48.84	ug/L	-0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.68%
21) 2-Butanone-d5	4.69	46	634881	126.57	ug/L	0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	126.57%
24) Chloroform-d	5.11	84	770829	66.36	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	132.72%#
26) 1,2-Dichloroethane-d4	5.74	65	531969	68.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	137.78%#
32) Benzene-d6	5.76	84	1560062	67.60	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	135.20%#
36) 1,2-Dichloropropane-d6	6.73	67	515445	68.68	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	137.36%#
41) Toluene-d8	7.93	98	1492341	68.37	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	136.74%#
43) trans-1,3-Dichloropropene-	8.21	79	274814	67.97	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	135.94%#
47) 2-Hexanone-d5	8.68	63	589522	153.28	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	153.28%#
57) 1,1,2,2-Tetrachloroethane-	10.79	84	815523	72.24	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	144.48%#
64) 1,2-Dichlorobenzene-d4	12.22	152	523724	67.36	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	134.72%#


Target Compounds					Ovalue
25) Chloroform	5.13	83	27737	2.363 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU011520\
Data File : VU036482.D
Acq On : 15 Jan 2020 21:19
Operator : JC/MD
Sample : L1118-12
Misc : 5.01G/5.0mL/100uL/5.0mL/MSVOA_U/METHANOL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GASK3

Quant Time: Jan 16 07:02:29 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 16 06:52:15 2020
Response via : Initial Calibration

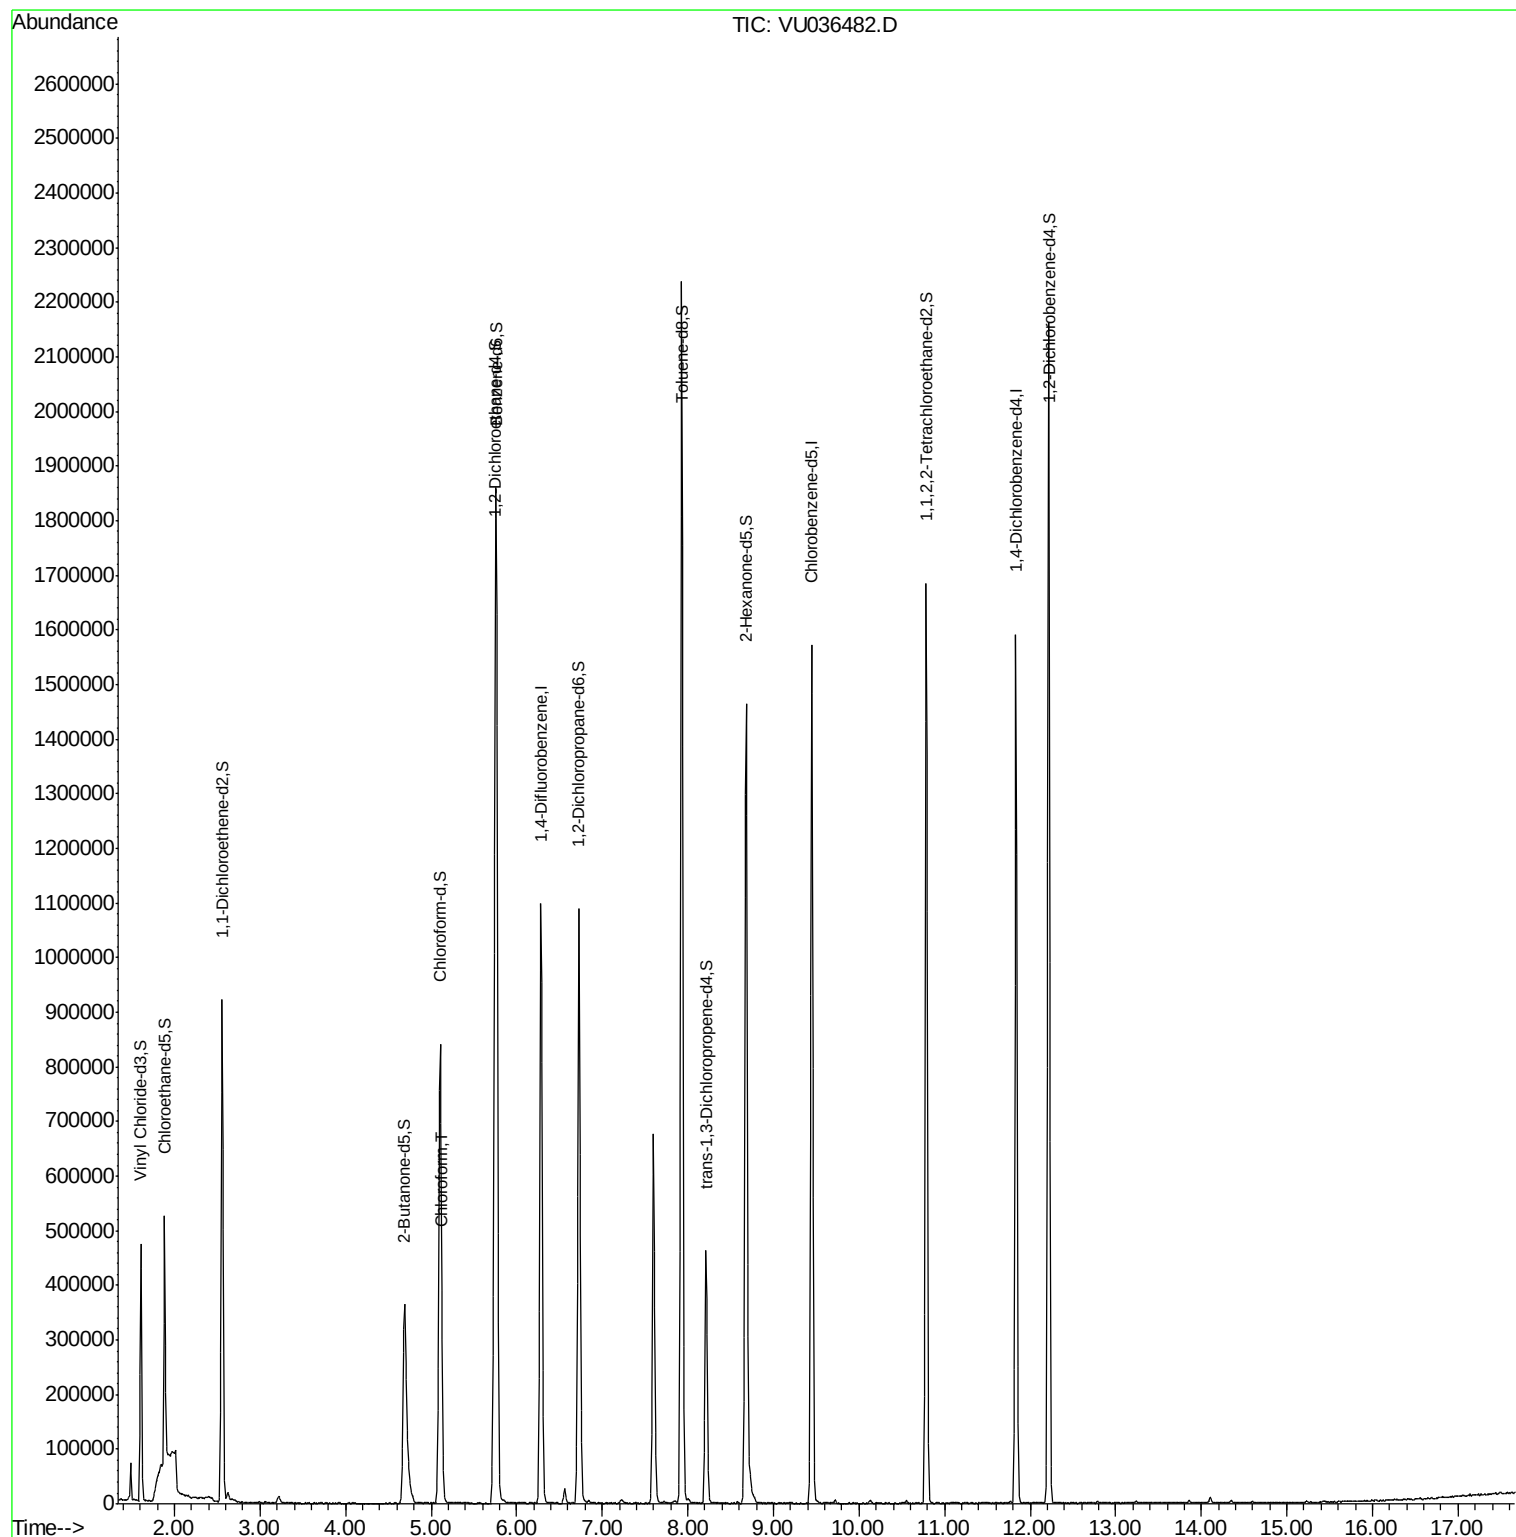

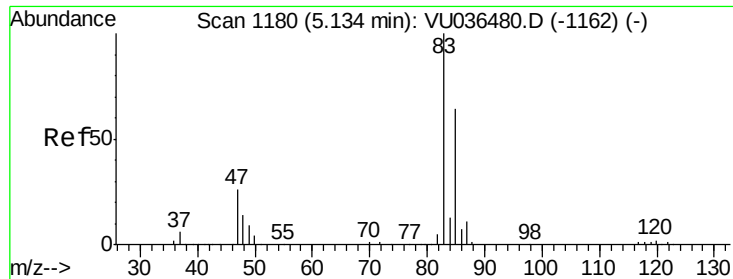

#25
 Chloroform
 Concen: 2.363 ug/L
 RT: 5.13 min Scan# 1180
 Delta R.T. -0.00 min
 Lab File: VU036482.D
 Acq: 15 Jan 2020 21:19

Instrument :
 MSVOA_U
 ClientSampleId :
 GASK3

Tot Ion: 83 Resp: 27737
 Ion Ratio Lower Upper
 83 100
 85 69.2 45.1 83.9

