


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU011520\
 Data File : VU036461.D
 Acq On : 15 Jan 2020 09:48
 Operator : JC/MD
 Sample : BFB40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB40

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
 Title : VOC Analysis
 Last Update : Thu Jan 16 14:14:58 2020

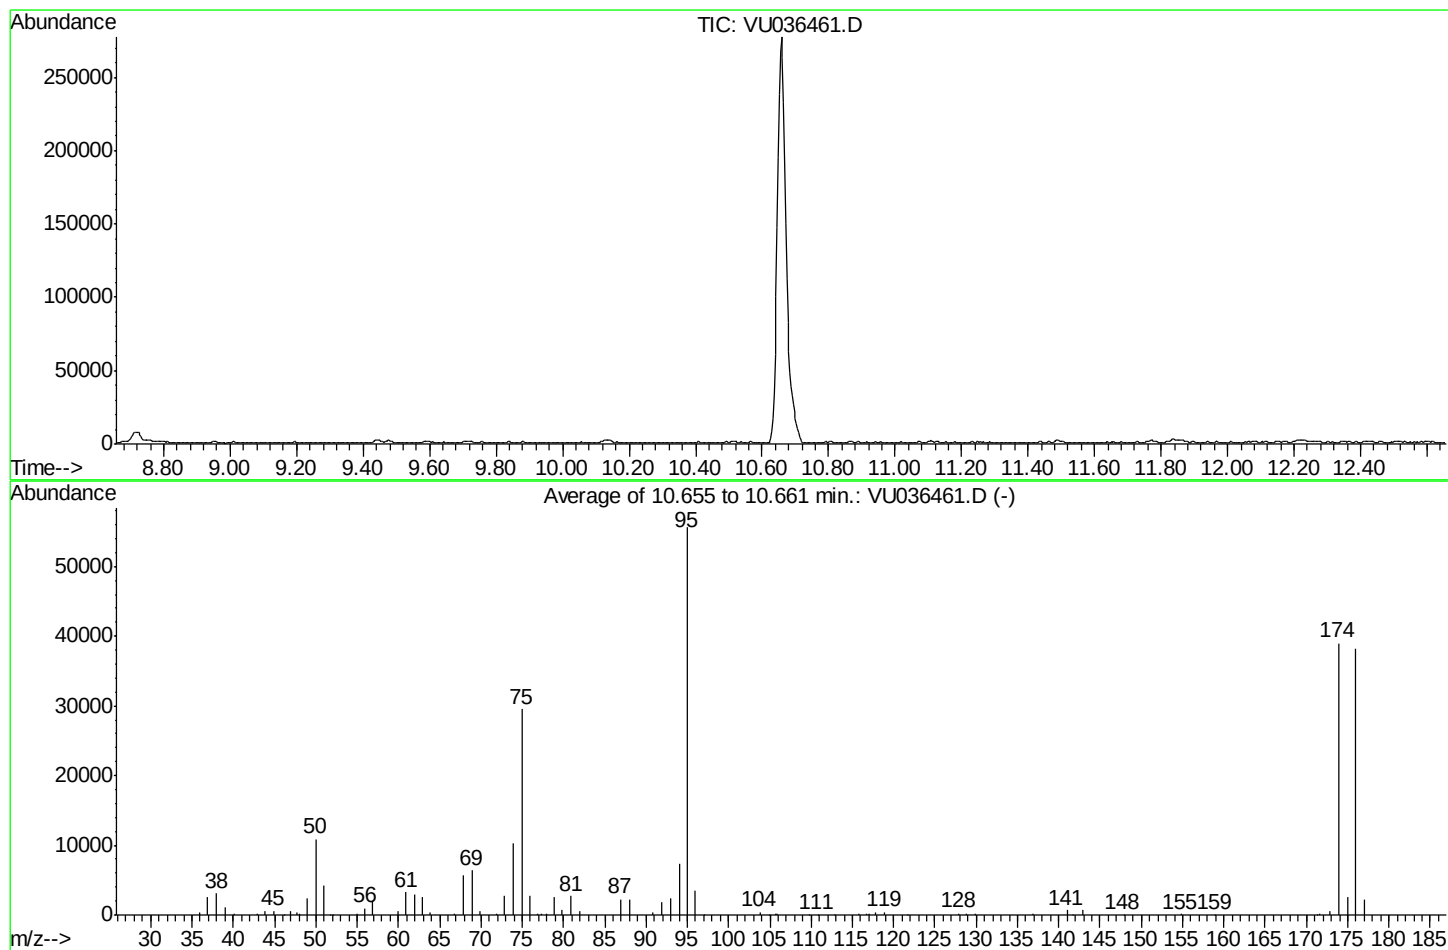

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	10926	PASS
75	95	30	80	53.1	29549	PASS
95	95	100	100	100.0	55613	PASS
96	95	5	9	6.3	3524	PASS
173	174	0.00	2	1.4	561	PASS
174	95	50	120	70.2	39021	PASS
175	174	5	9	6.8	2642	PASS
176	174	95	101	97.7	38136	PASS
177	176	5	9	5.7	2186	PASS

m/z	Abundance
35.80	372.0
36.90	2707.0
37.90	2954.0
38.90	1231.0
40.10	139.0
42.90	116.0
43.80	1137.0
45.00	622.0
46.20	144.0
47.10	514.0
47.70	294.0
48.10	289.0
48.90	2528.0
50.00	10792.0
50.90	3820.0
52.10	130.0
55.00	162.0
56.00	923.0
56.90	2014.0
60.00	585.0
60.90	3122.0
62.00	2828.0
62.90	2914.0
63.90	291.0
66.90	212.0
67.90	5782.0
69.00	6477.0
69.90	626.0
71.90	194.0
72.90	2783.0
74.00	10502.0
75.00	29816.0
75.90	2848.0
76.80	185.0
77.40	161.0
78.80	2752.0
79.80	800.0
80.90	2546.0
81.90	778.0
86.90	2282.0
87.90	2028.0
90.80	347.0
91.90	1636.0
93.00	2332.0
94.00	7644.0
95.00	54656.0
96.00	3523.0
103.80	371.0
105.70	304.0
109.80	120.0
110.70	137.0
112.90	103.0
115.80	252.0
117.00	283.0
117.80	321.0
118.90	455.0
127.90	258.0
129.00	110.0
129.90	132.0
136.90	206.0
141.00	703.0
141.70	108.0
143.00	777.0
147.80	145.0
154.80	162.0
171.70	155.0
172.90	659.0
173.90	38920.0
175.00	3016.0
176.00	36472.0
177.00	2089.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
35.90	453.0
36.90	2565.0
38.00	3210.0
38.90	1221.0
40.10	120.0
42.90	121.0
43.80	1028.0
44.90	566.0
46.20	126.0
47.00	524.0
47.70	299.0
48.00	276.0
48.90	2536.0
50.00	11225.0
50.90	4316.0
51.80	105.0
54.90	197.0
55.90	1005.0
56.90	1958.0
59.90	677.0
61.00	3360.0
62.00	2938.0
62.90	2717.0
63.90	310.0
66.90	223.0
67.90	5681.0
68.90	6473.0
69.90	562.0
72.00	217.0
73.00	2976.0
73.90	10597.0
75.00	30216.0
75.90	2894.0
76.80	196.0
77.40	135.0
77.90	187.0
78.80	2712.0
79.80	797.0
80.90	2792.0
81.90	667.0
86.90	2368.0
87.90	2247.0
90.90	429.0
91.90	1772.0
93.00	2471.0
94.00	7478.0
95.00	57432.0
96.00	3658.0
97.00	123.0
103.80	401.0
105.90	314.0
109.80	103.0
110.80	126.0
115.80	260.0
116.70	247.0
117.00	266.0
117.70	398.0
118.90	446.0
121.70	115.0
127.90	294.0
128.80	103.0
129.90	119.0
136.90	201.0
141.10	763.0
142.90	701.0
154.80	167.0
158.90	103.0
171.60	160.0
172.80	603.0
173.90	40296.0
174.90	2672.0
176.00	39360.0
176.90	2208.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
35.90	499.0
36.90	2340.0
38.00	3150.0
39.00	1132.0
40.00	139.0
42.80	111.0
43.90	1069.0
44.80	505.0
46.90	527.0
47.70	259.0
48.00	268.0
48.90	2215.0
50.00	10761.0
50.90	4330.0
51.80	119.0
54.90	240.0
55.90	1077.0
56.90	1845.0
59.90	594.0
61.00	3183.0
62.00	2916.0
62.90	2287.0
63.90	289.0
66.80	215.0
67.90	5526.0
68.90	6091.0
69.90	472.0
71.90	316.0
73.00	3112.0
73.90	9730.0
75.00	28616.0
75.90	2672.0
76.90	238.0
77.90	255.0
78.80	2405.0
79.80	725.0
80.90	2797.0
81.90	496.0
86.90	2245.0
88.00	2268.0
90.90	435.0
91.90	1894.0
93.00	2573.0
94.00	6938.0
95.00	54752.0
96.00	3392.0
103.80	385.0
104.90	167.0
105.90	347.0
115.80	209.0
116.70	292.0
117.70	454.0
118.90	364.0
127.90	227.0
128.80	141.0
129.90	138.0
136.90	149.0
141.10	704.0
142.90	628.0
154.80	171.0
158.90	120.0
171.30	155.0
172.90	423.0
173.90	37848.0
175.00	2238.0
176.00	38576.0
176.90	2261.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

Scan 2885 (10.616 min): VU036461.D
BFB40

m/z	Abundance
39.80	153.0
43.70	535.0
72.90	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40