

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
 Data File : VU042062.D
 Acq On : 15 Jan 2021 10:49
 Operator : SY/MD
 Sample : M1049-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Quant Time: Jan 16 01:07:05 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jan 16 01:05:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.260	114	133810	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	132127	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.809	152	57871	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	41215	4.08	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.60%
7) Chloroethane-d5	1.919	69	44188	4.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.40%
11) 1,1-Dichloroethene-d2	2.575	63	62636	3.08	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.60%
20) 2-Butanone-d5	4.658	46	172530	50.92	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.84%
24) Chloroform-d	5.076	84	101800	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
26) 1,2-Dichloroethane-d4	5.713	65	57869	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.80%
32) Benzene-d6	5.739	84	192962	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.40%
36) 1,2-Dichloropropane-d6	6.700	67	66180	4.72	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.40%
41) Toluene-d8	7.903	98	157409	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.40%
43) trans-1,3-Dichloroprop...	8.182	79	24184	4.30	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.00%
46) 2-Hexanone-d5	8.642	63	145109	50.27	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.54%
57) 1,1,2,2-Tetrachloroeth...	10.755	84	59521	5.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	111.60%
64) 1,2-Dichlorobenzene-d4	12.189	152	57206	5.25	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.00%
Target Compounds						Qvalue
16) Methylene chloride	3.057	84	1982	0.16	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
Data File : VU042062.D
Acq On : 15 Jan 2021 10:49
Operator : SY/MD
Sample : M1049-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Jan 16 01:07:05 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jan 16 01:05:16 2021
Response via : Initial Calibration

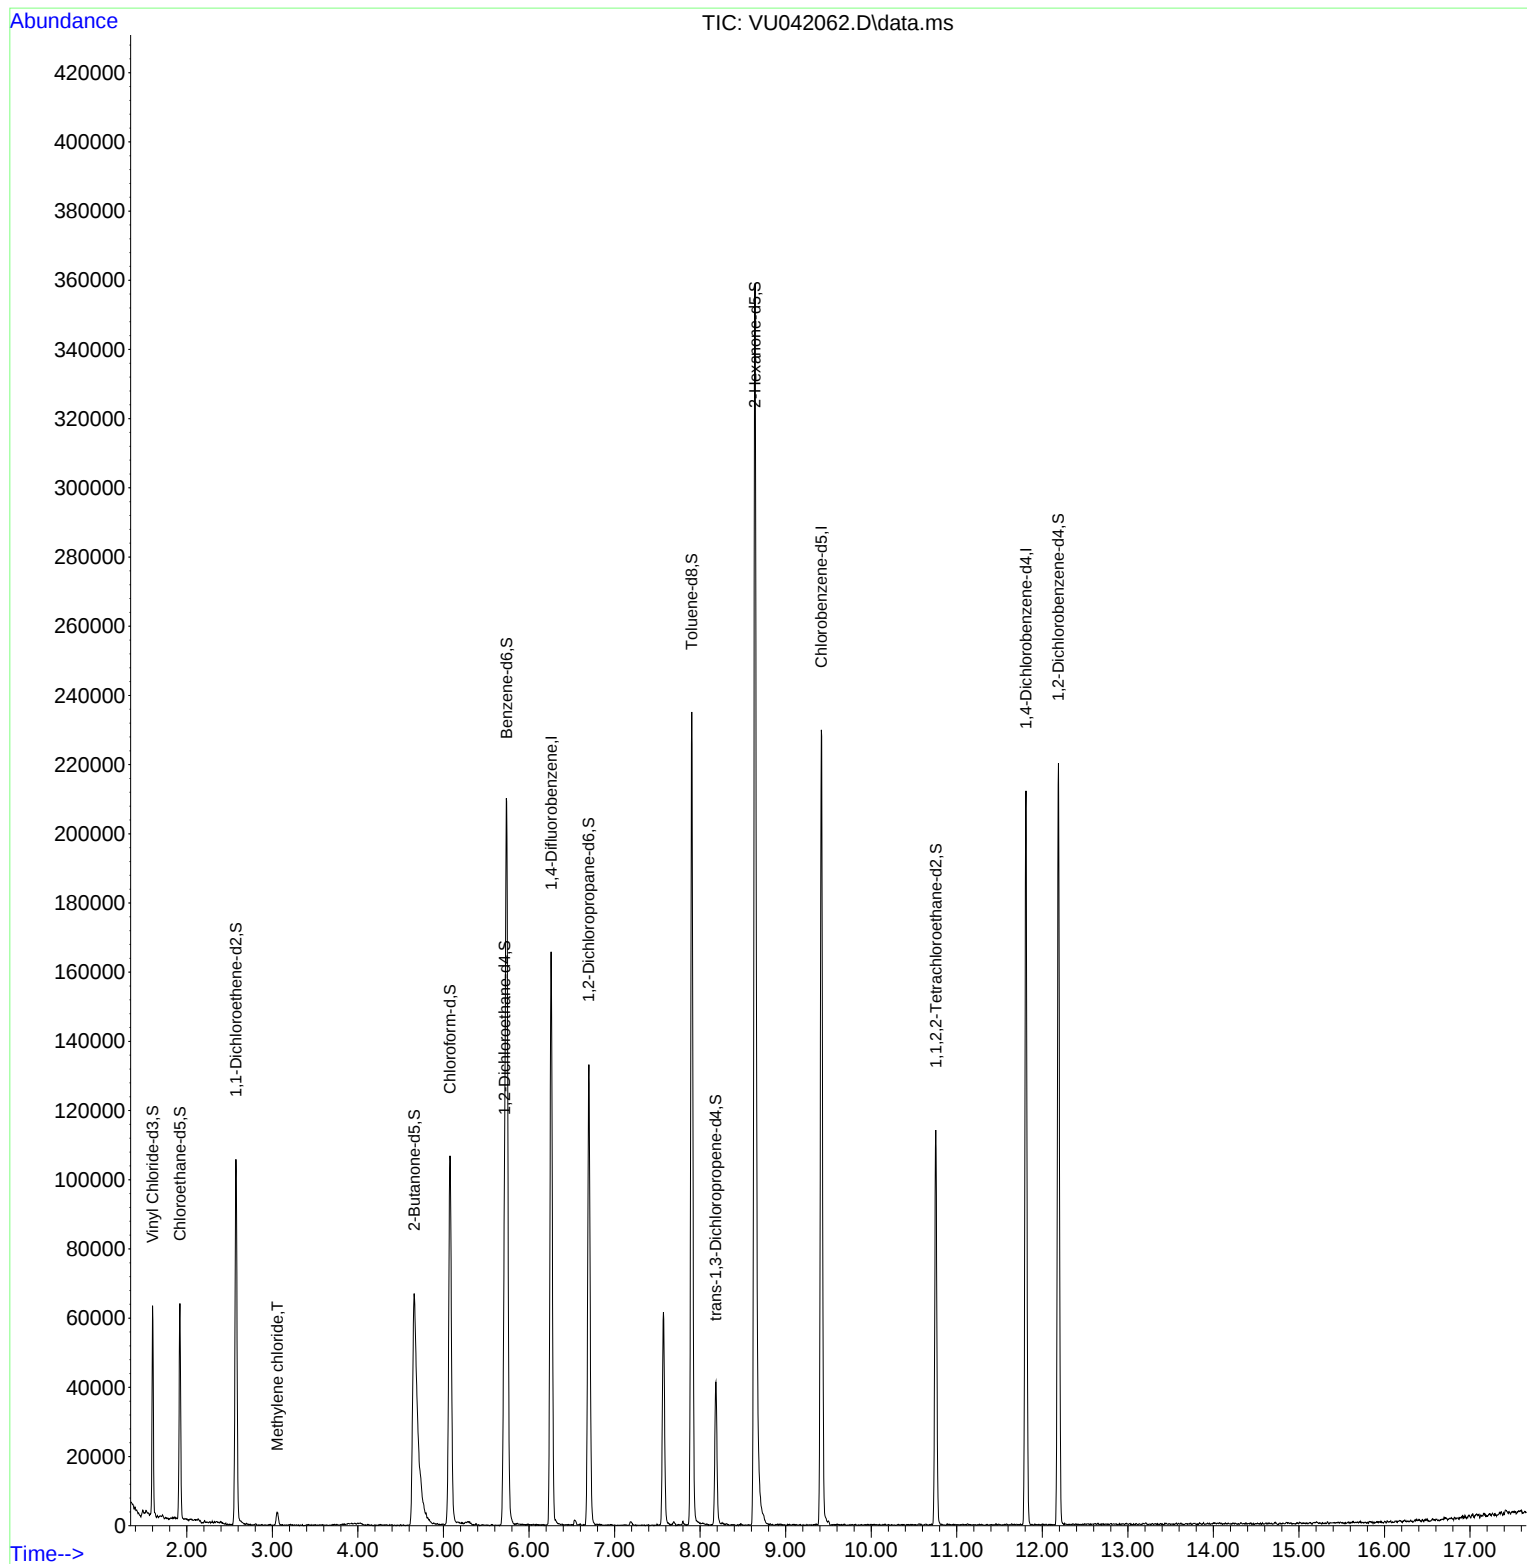

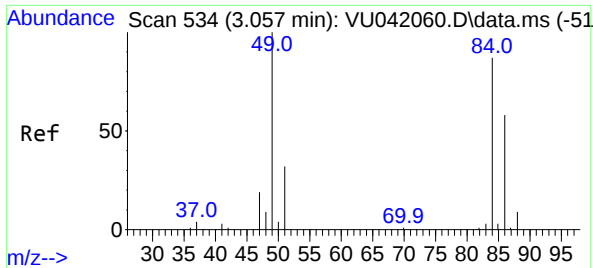

#16
Methylene chloride
Concen: 0.16 ug/L
RT: 3.057 min Scan# 534
Delta R.T. 0.000 min
Lab File: VU042062.D
Acq: 15 Jan 2021 10:49

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Tgt Ion:	84	Resp:	1982
Ion	Ratio	Lower	Upper
84	100		
86	48.7	42.6	79.0
49	107.1	86.2	160.0

