

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
 Data File : VU042070.D
 Acq On : 15 Jan 2021 14:01
 Operator : SY/MD
 Sample : M1065-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXS2

Quant Time: Jan 16 01:10:05 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jan 16 01:05:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.260	114	121144	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	122560	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.809	152	56149	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	38149	4.17	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.40%
7) Chloroethane-d5	1.919	69	43259	5.00	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.00%
11) 1,1-Dichloroethene-d2	2.575	63	61668	3.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.00%
20) 2-Butanone-d5	4.649	46	166801	54.37	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.74%
24) Chloroform-d	5.079	84	102547	5.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.60%
26) 1,2-Dichloroethane-d4	5.716	65	49340	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
32) Benzene-d6	5.742	84	161372	4.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.40%
36) 1,2-Dichloropropane-d6	6.703	67	55236	4.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.00%
41) Toluene-d8	7.903	98	134825	3.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.20%
43) trans-1,3-Dichloroprop...	8.185	79	21807	4.18	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.60%
46) 2-Hexanone-d5	8.642	63	120605	45.04	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.08%
57) 1,1,2,2-Tetrachloroeth...	10.755	84	47915	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.80%
64) 1,2-Dichlorobenzene-d4	12.189	152	51143	4.84	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.80%
Target Compounds						
13) Acetone	2.655	43	14660	7.65	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
Data File : VU042070.D
Acq On : 15 Jan 2021 14:01
Operator : SY/MD
Sample : M1065-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXS2

Quant Time: Jan 16 01:10:05 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jan 16 01:05:16 2021
Response via : Initial Calibration

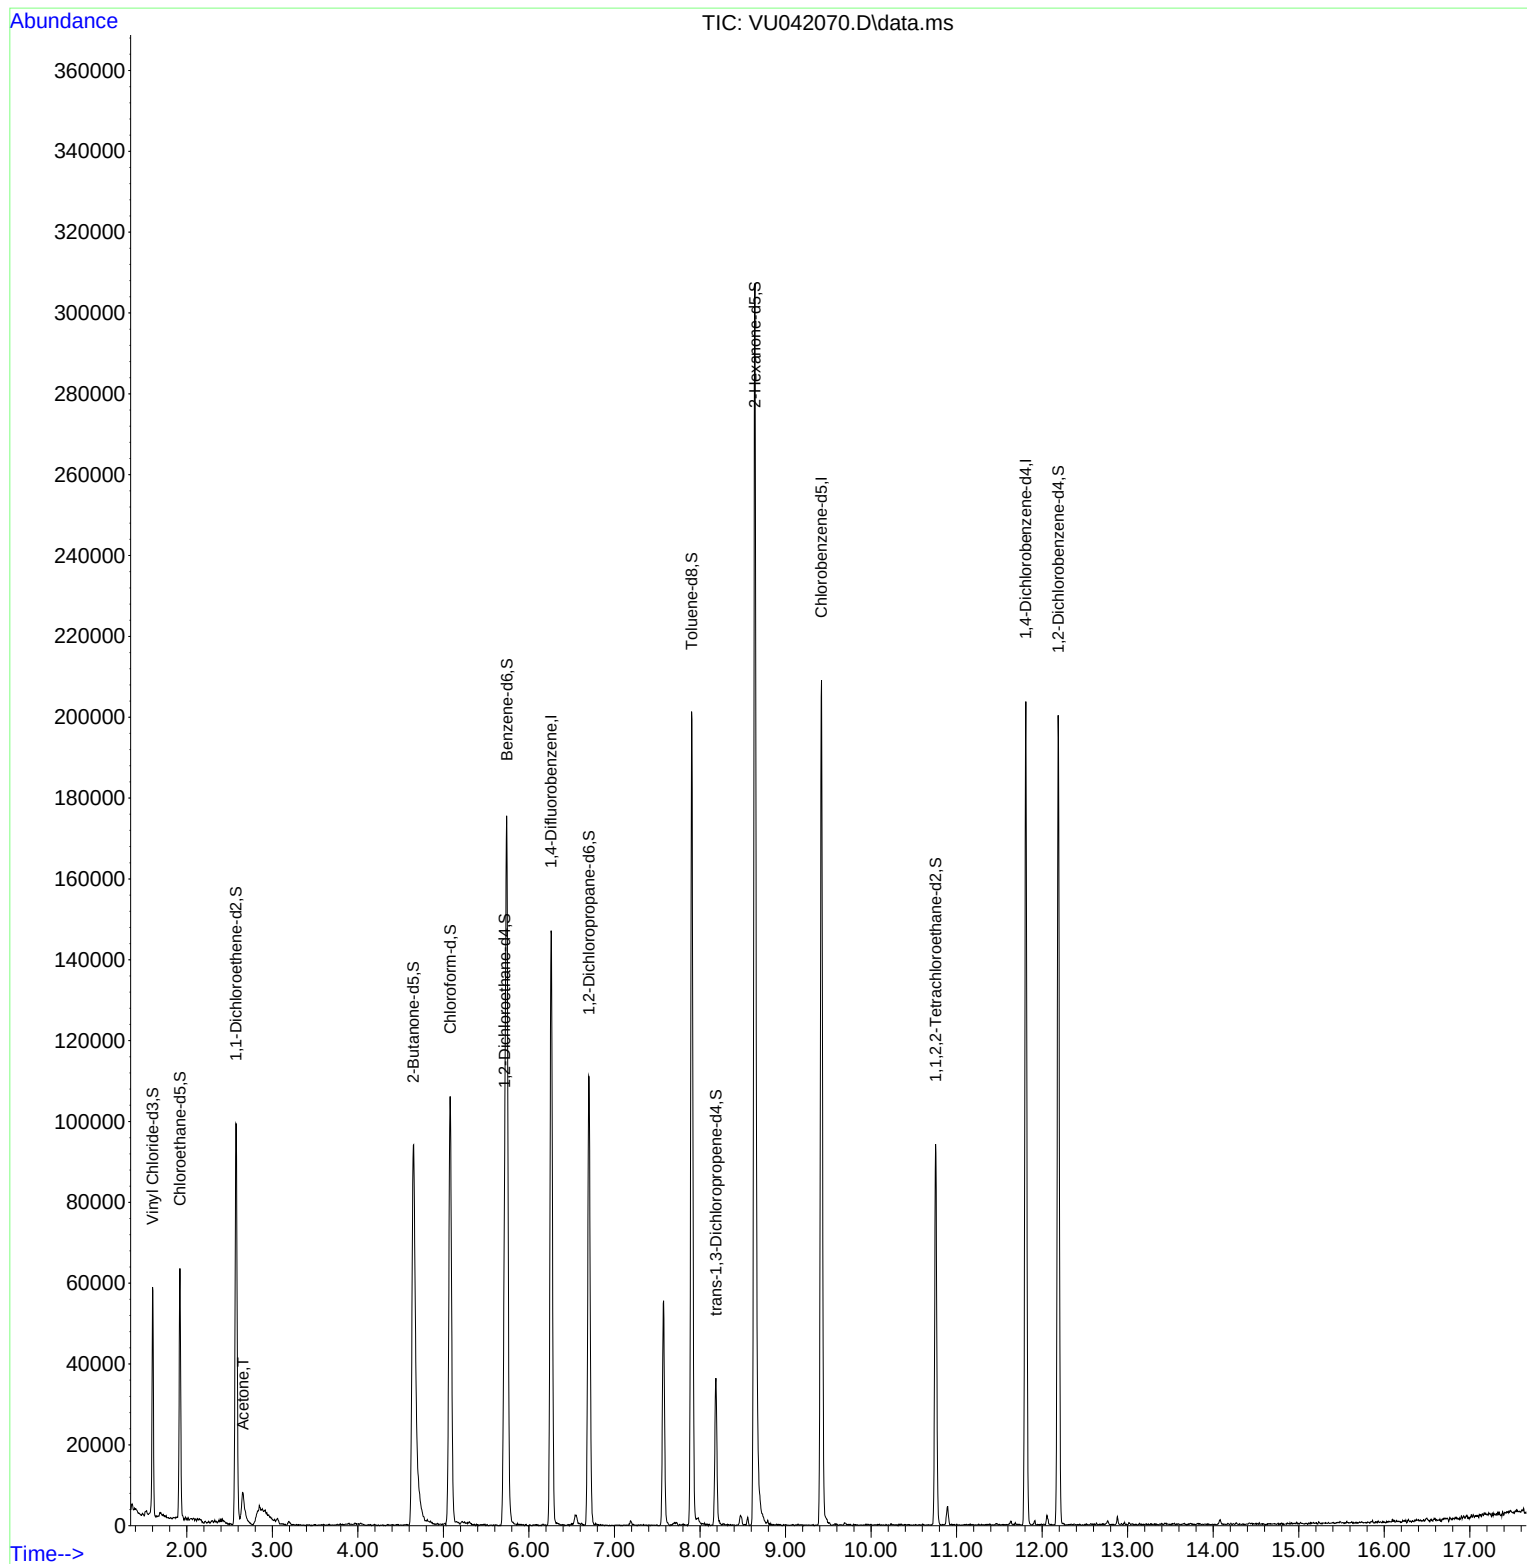

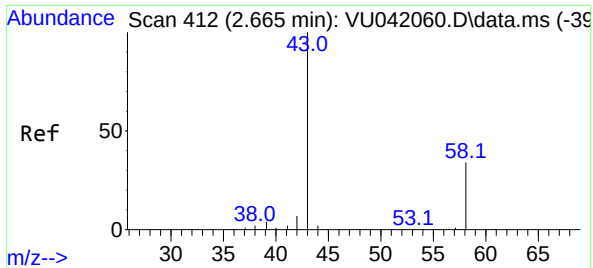

#13
Acetone
Concen: 7.65 ug/L
RT: 2.655 min Scan# 409
Delta R.T. -0.010 min
Lab File: VU042070.D
Acq: 15 Jan 2021 14:01

Instrument :
MSVOA_U
ClientSampleId :
BFXS2

Tgt Ion:	43	Resp:	14660
Ion	Ratio	Lower	Upper
43	100		
58	33.4	0.0	57.4

