

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
 Data File : VU042080.D
 Acq On : 15 Jan 2021 18:26
 Operator : SY/MD
 Sample : M1065-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Quant Time: Jan 16 01:13:55 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jan 16 01:05:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.259	114	134410	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	108462	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.809	152	49285	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	35641	3.51	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	70.20%
7) Chloroethane-d5	1.919	69	42467	4.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.40%
11) 1,1-Dichloroethene-d2	2.575	63	61227	3.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.00%
20) 2-Butanone-d5	4.655	46	189437	55.66	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.32%
24) Chloroform-d	5.079	84	103488	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.60%
26) 1,2-Dichloroethane-d4	5.716	65	59777	5.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.60%
32) Benzene-d6	5.742	84	196090	5.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.80%
36) 1,2-Dichloropropane-d6	6.700	67	66359	5.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	115.40%
41) Toluene-d8	7.906	98	132063	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.20%
43) trans-1,3-Dichloroprop...	8.185	79	21978	4.76	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.20%
46) 2-Hexanone-d5	8.642	63	135669	57.26	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	114.52%
57) 1,1,2,2-Tetrachloroeth...	10.754	84	50969	5.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	116.40%
64) 1,2-Dichlorobenzene-d4	12.188	152	51368	5.53	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.60%
Target Compounds						Qvalue
16) Methylene chloride	3.057	84	1950	0.16	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
Data File : VU042080.D
Acq On : 15 Jan 2021 18:26
Operator : SY/MD
Sample : M1065-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Jan 16 01:13:55 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jan 16 01:05:16 2021
Response via : Initial Calibration

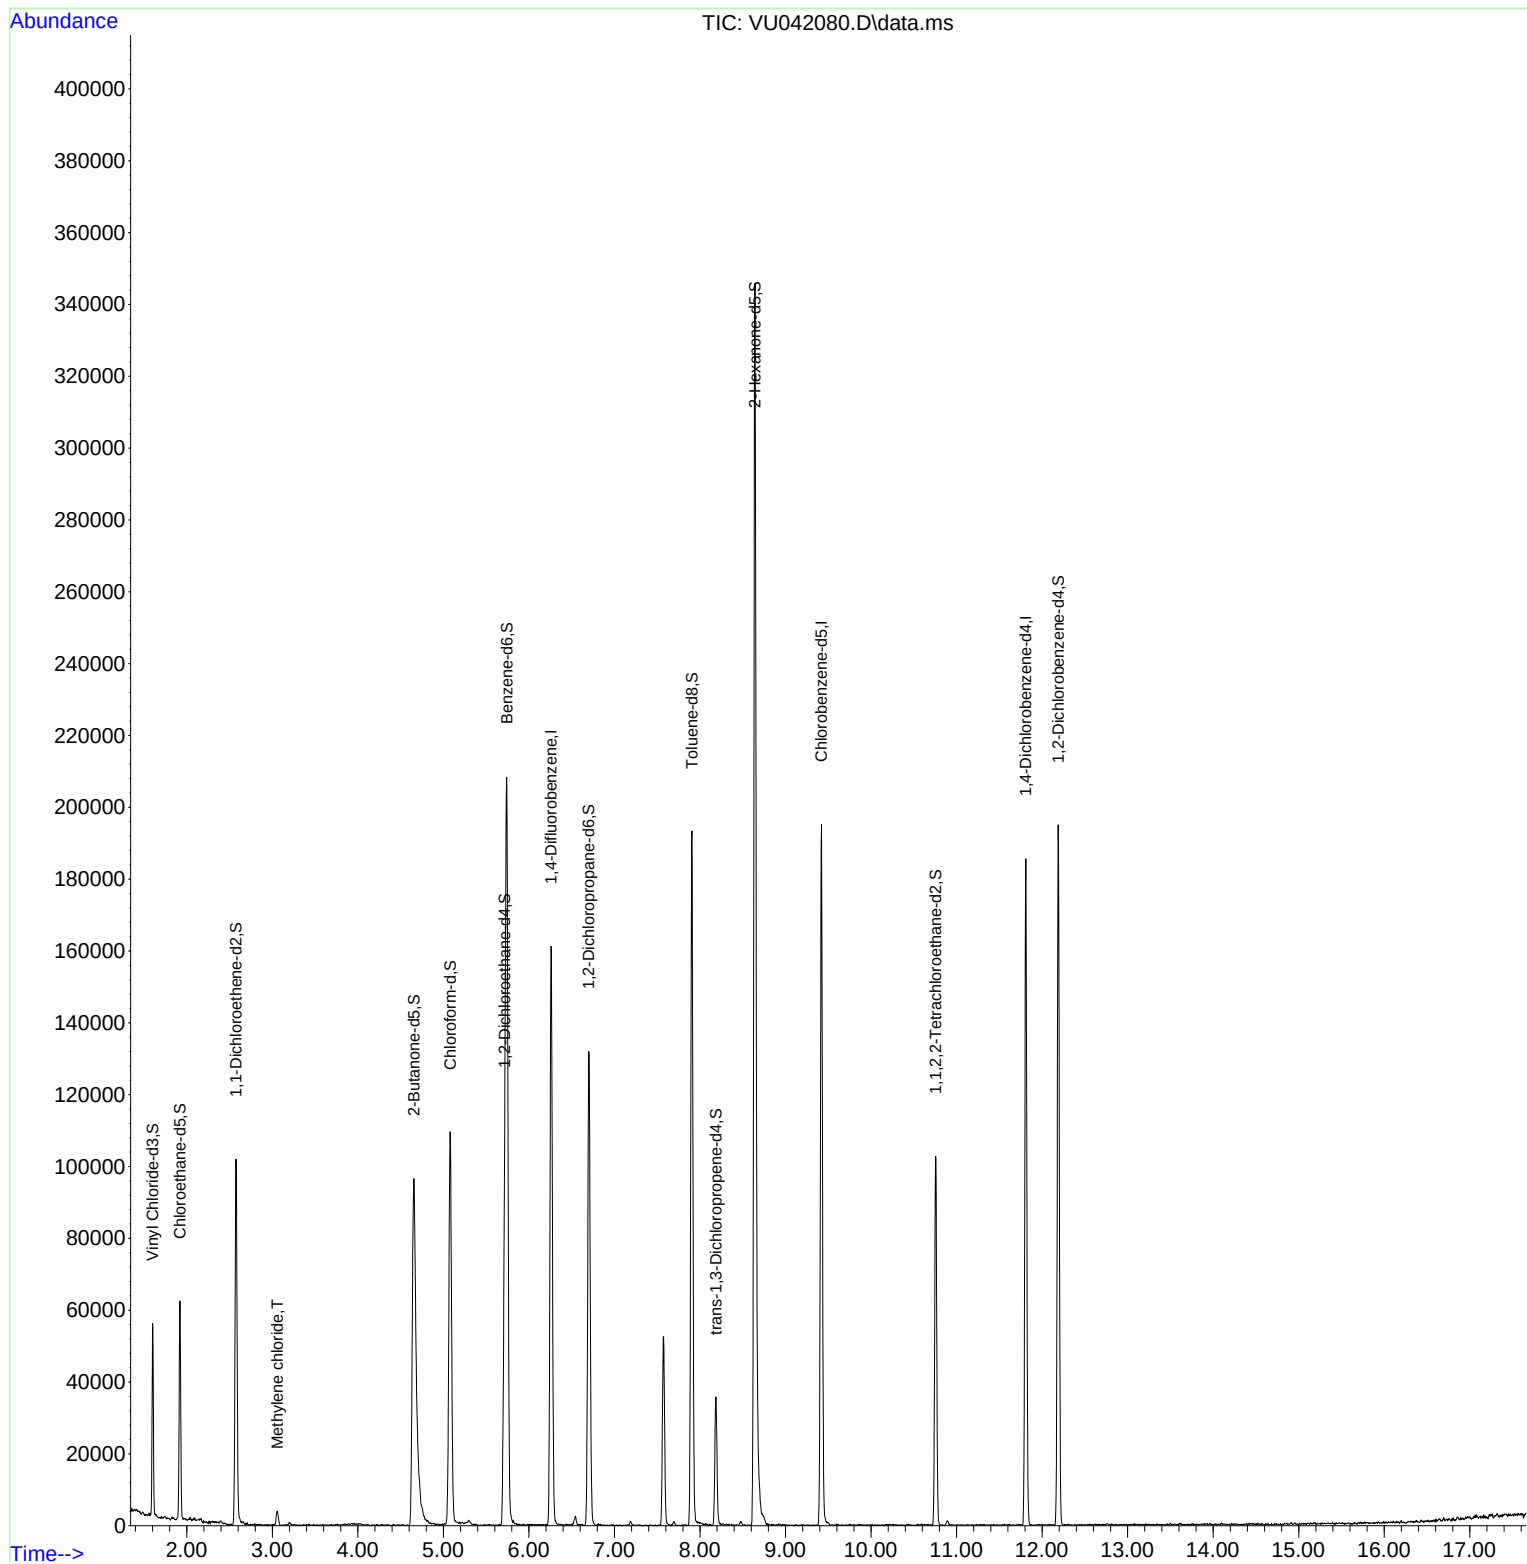

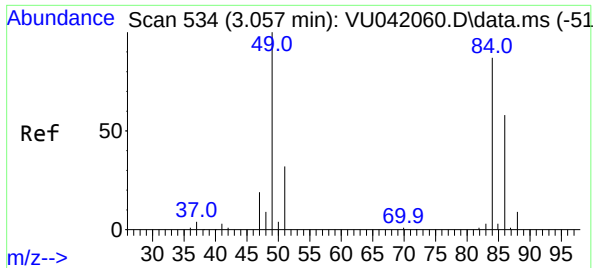

#16
Methylene chloride
Concen: 0.16 ug/L
RT: 3.057 min Scan# 534
Delta R.T. -0.000 min
Lab File: VU042080.D
Acq: 15 Jan 2021 18:26

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Tgt Ion:	84	Resp:	1950
Ion	Ratio	Lower	Upper
84	100		
86	68.5	42.6	79.0
49	105.7	86.2	160.0

