

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
 Data File : VU042075.D
 Acq On : 15 Jan 2021 16:01
 Operator : SY/MD
 Sample : M1065-06DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXN2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC: VU042075.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	95	rVB	57385	61083	8.89%	1.430%
2	1.919	170	180	192	rBV	62882	77670	11.30%	1.819%
3	2.578	373	385	402	rBV	100565	165826	24.13%	3.883%
4	3.057	525	534	550	rVB2	4636	8160	1.19%	0.191%
5	4.652	1011	1030	1073	rBV	84580	276402	40.22%	6.472%
6	5.079	1147	1163	1182	rBV	93127	202116	29.41%	4.733%
7	5.738	1348	1368	1390	rBV3	171973	447131	65.07%	10.470%
8	6.259	1516	1530	1553	rBV	145646	275475	40.09%	6.450%
9	6.552	1604	1621	1640	rVB	94256	177421	25.82%	4.154%
10	6.703	1654	1668	1688	rVB	110274	214295	31.19%	5.018%
11	7.574	1925	1939	1953	rBV	53900	93519	13.61%	2.190%
12	7.906	2028	2042	2057	rBV	202919	343731	50.02%	8.049%
13	8.185	2118	2129	2143	rBV2	35142	59348	8.64%	1.390%
14	8.555	2235	2244	2255	rVB3	22530	36881	5.37%	0.864%
15	8.642	2255	2271	2303	rBV	354608	687172	100.00%	16.090%
16	9.420	2500	2513	2540	rBV	210366	347913	50.63%	8.147%
17	10.754	2917	2928	2944	rVB	93989	151413	22.03%	3.545%
18	11.809	3244	3256	3273	rVB	202291	321609	46.80%	7.531%
19	12.188	3362	3374	3391	rVB	200186	323537	47.08%	7.576%




Sum of corrected areas: 4270702

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
Data File : VU042075.D
Acq On : 15 Jan 2021 16:01
Operator : SY/MD
Sample : M1065-06DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXN2DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

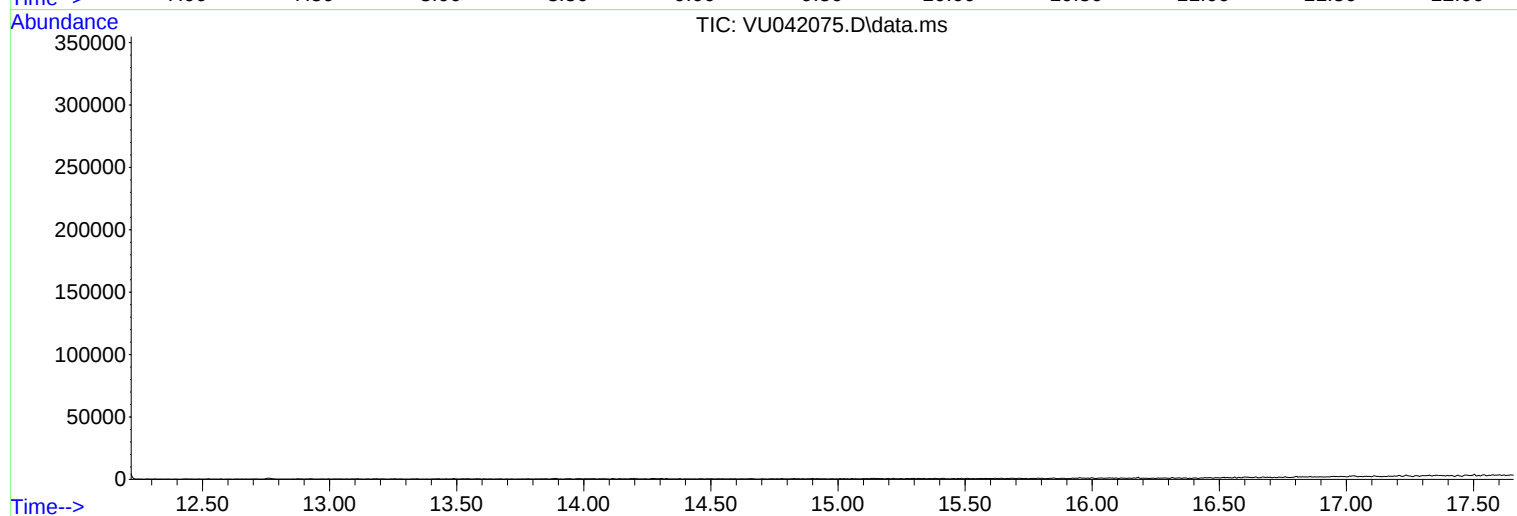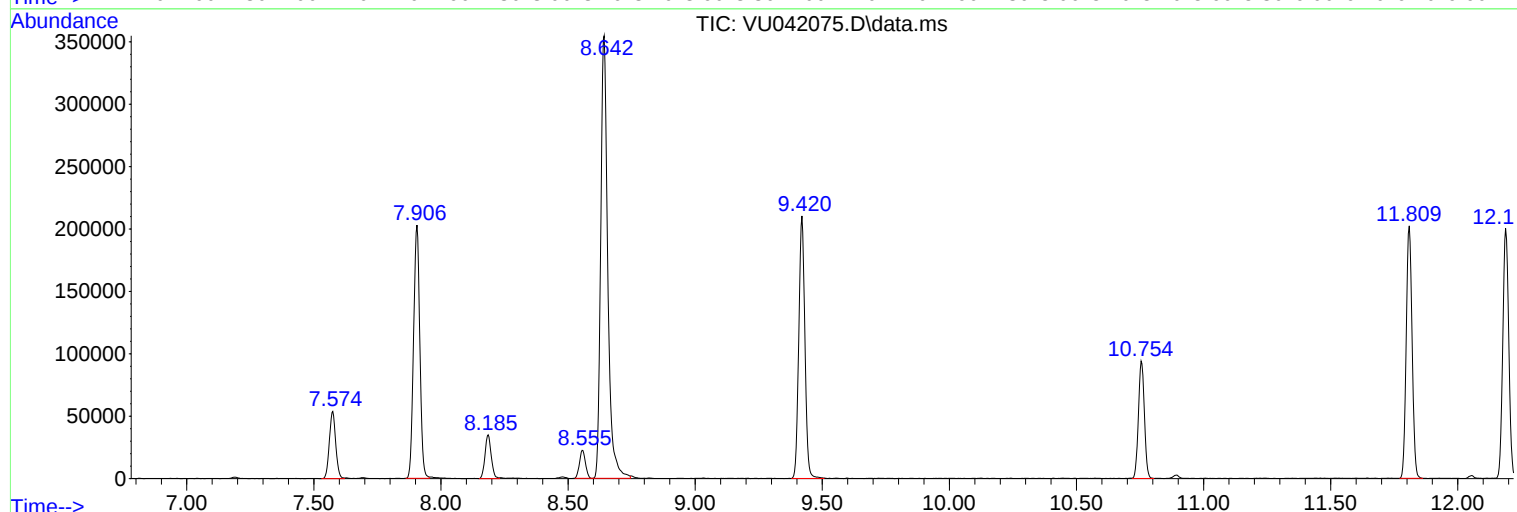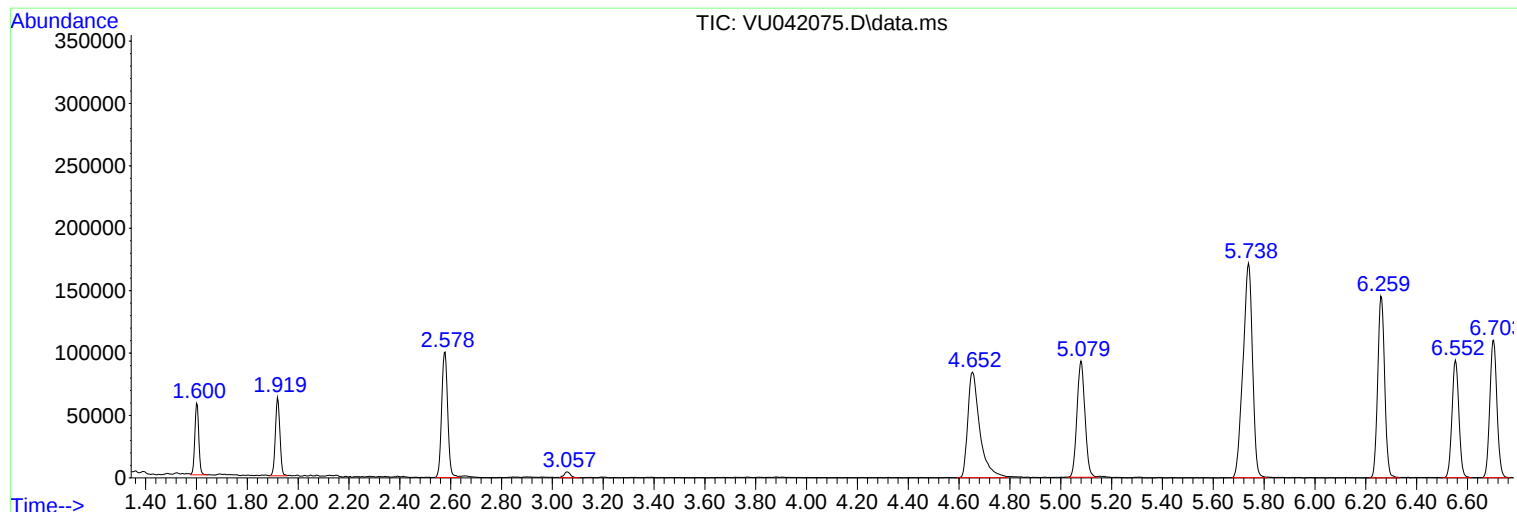

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
Data File : VU042075.D
Acq On : 15 Jan 2021 16:01
Operator : SY/MD
Sample : M1065-06DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXN2DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
Data File : VU042075.D
Acq On : 15 Jan 2021 16:01
Operator : SY/MD
Sample : M1065-06DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXN2DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
