

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
 Data File : VU042078.D
 Acq On : 15 Jan 2021 17:38
 Operator : SY/MD
 Sample : M1065-16DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXP6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC: VU042078.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	90	rBV	49703	53596	6.63%	1.171%
2	1.919	171	180	193	rVB	59448	73520	9.10%	1.607%
3	2.575	371	384	399	rBV	96803	157759	19.52%	3.447%
4	3.057	525	534	548	rVB2	8345	15568	1.93%	0.340%
5	4.655	1014	1031	1059	rBV	99121	331003	40.96%	7.233%
6	5.080	1145	1163	1182	rBV	93434	209420	25.91%	4.576%
7	5.739	1344	1368	1389	rBV2	179443	470652	58.24%	10.285%
8	6.260	1516	1530	1550	rBV	155030	281749	34.86%	6.157%
9	6.555	1606	1622	1640	rBV2	127246	247518	30.63%	5.409%
10	6.703	1654	1668	1687	rBV	115019	224766	27.81%	4.912%
11	7.571	1926	1938	1953	rBV	57437	100002	12.37%	2.185%
12	7.906	2028	2042	2059	rBV	204847	353538	43.74%	7.726%
13	8.186	2117	2129	2141	rBV	39896	65852	8.15%	1.439%
14	8.559	2234	2245	2257	rBV2	35480	59852	7.41%	1.308%
15	8.642	2257	2271	2299	rBV	425119	808180	100.00%	17.661%
16	9.420	2499	2513	2536	rBV	221415	371061	45.91%	8.109%
17	10.755	2915	2928	2944	rVB	99412	161232	19.95%	3.523%
18	11.809	3244	3256	3272	rBV	176901	281368	34.82%	6.149%
19	12.189	3362	3374	3391	rBV	191012	309422	38.29%	6.762%




Sum of corrected areas: 4576058

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
Data File : VU042078.D
Acq On : 15 Jan 2021 17:38
Operator : SY/MD
Sample : M1065-16DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXP6DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

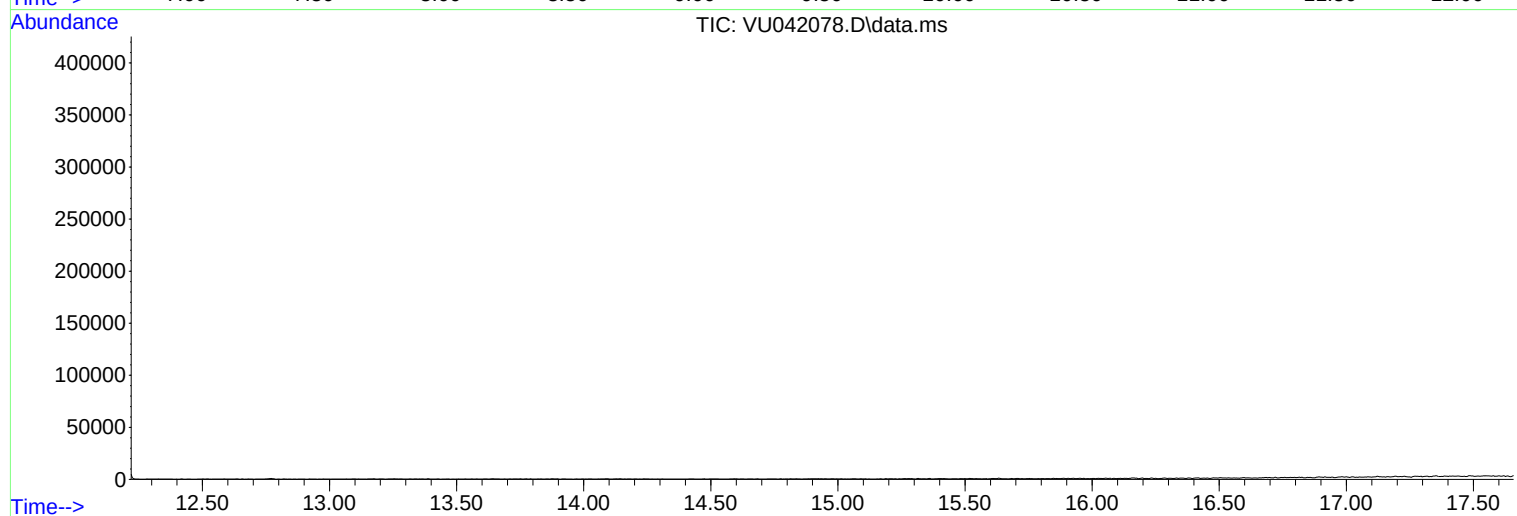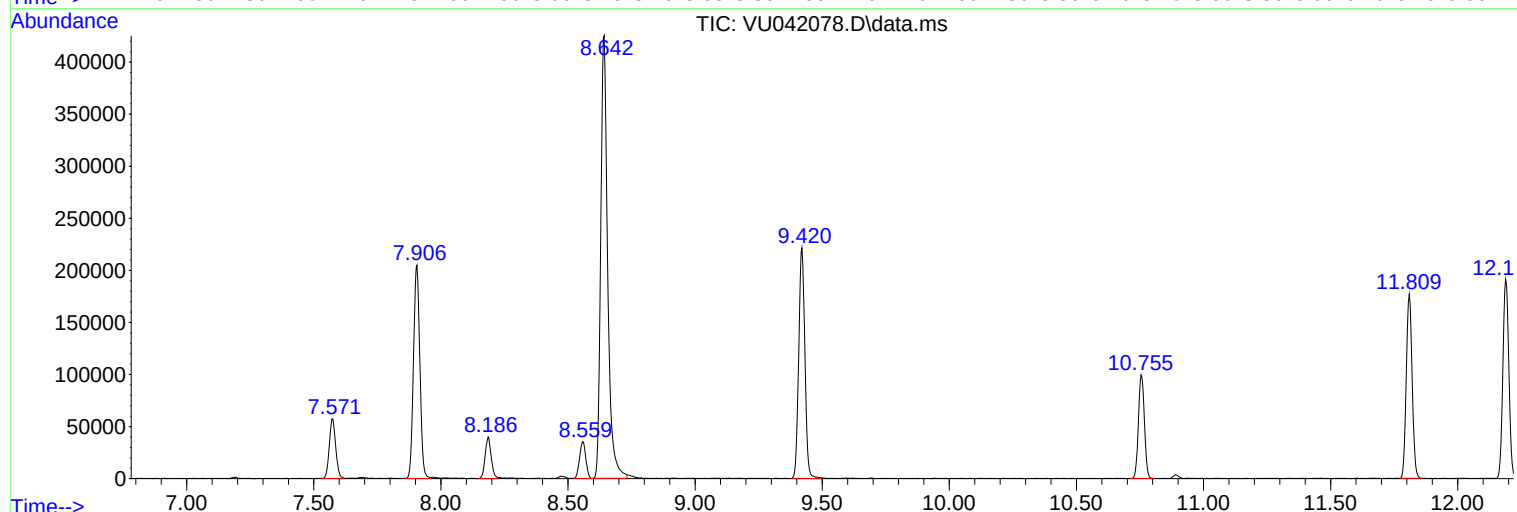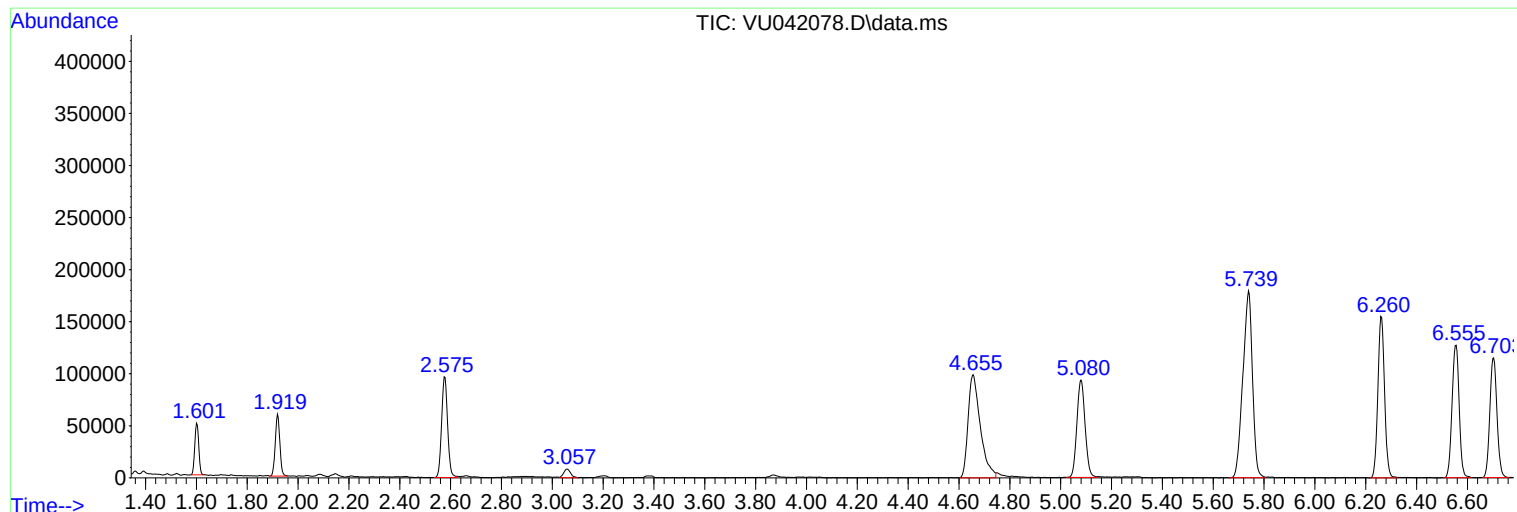

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
Data File : VU042078.D
Acq On : 15 Jan 2021 17:38
Operator : SY/MD
Sample : M1065-16DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXP6DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
Data File : VU042078.D
Acq On : 15 Jan 2021 17:38
Operator : SY/MD
Sample : M1065-16DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXP6DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
