

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
 Data File : VU042084.D
 Acq On : 15 Jan 2021 20:02
 Operator : SY/MD
 Sample : M1164-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXQ0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC: VU042084.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.388	8	15	25	rBV	22600	22460	2.84%	0.493%
2	1.600	74	81	93	rVB	52631	57124	7.21%	1.253%
3	1.919	171	180	190	rVB	60880	73896	9.33%	1.621%
4	2.144	241	250	264	rVB	12536	19603	2.47%	0.430%
5	2.575	373	384	398	rBV	98605	158319	19.99%	3.473%
6	4.655	1015	1031	1079	rBV	92442	335076	42.30%	7.351%
7	5.079	1145	1163	1185	rBV2	107022	235346	29.71%	5.163%
8	5.739	1345	1368	1388	rBV2	203752	538747	68.01%	11.819%
9	6.259	1516	1530	1554	rBV	160122	302928	38.24%	6.646%
10	6.552	1609	1621	1636	rBV2	25404	48893	6.17%	1.073%
11	6.703	1654	1668	1688	rBV2	128280	253351	31.98%	5.558%
12	7.575	1925	1939	1956	rBV	62108	111556	14.08%	2.447%
13	7.906	2028	2042	2059	rBV	227049	396136	50.01%	8.690%
14	8.185	2118	2129	2144	rBV	44995	74800	9.44%	1.641%
15	8.558	2235	2245	2255	rBV2	19124	32011	4.04%	0.702%
16	8.642	2257	2271	2300	rBV	406394	792153	100.00%	17.378%
17	9.420	2499	2513	2534	rBV	210536	347039	43.81%	7.613%
18	10.754	2915	2928	2942	rBV	97593	157968	19.94%	3.465%
19	11.809	3243	3256	3273	rBV	181638	291073	36.74%	6.385%
20	12.188	3361	3374	3390	rBV	191033	309875	39.12%	6.798%




Sum of corrected areas: 4558354

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
Data File : VU042084.D
Acq On : 15 Jan 2021 20:02
Operator : SY/MD
Sample : M1164-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXQ0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

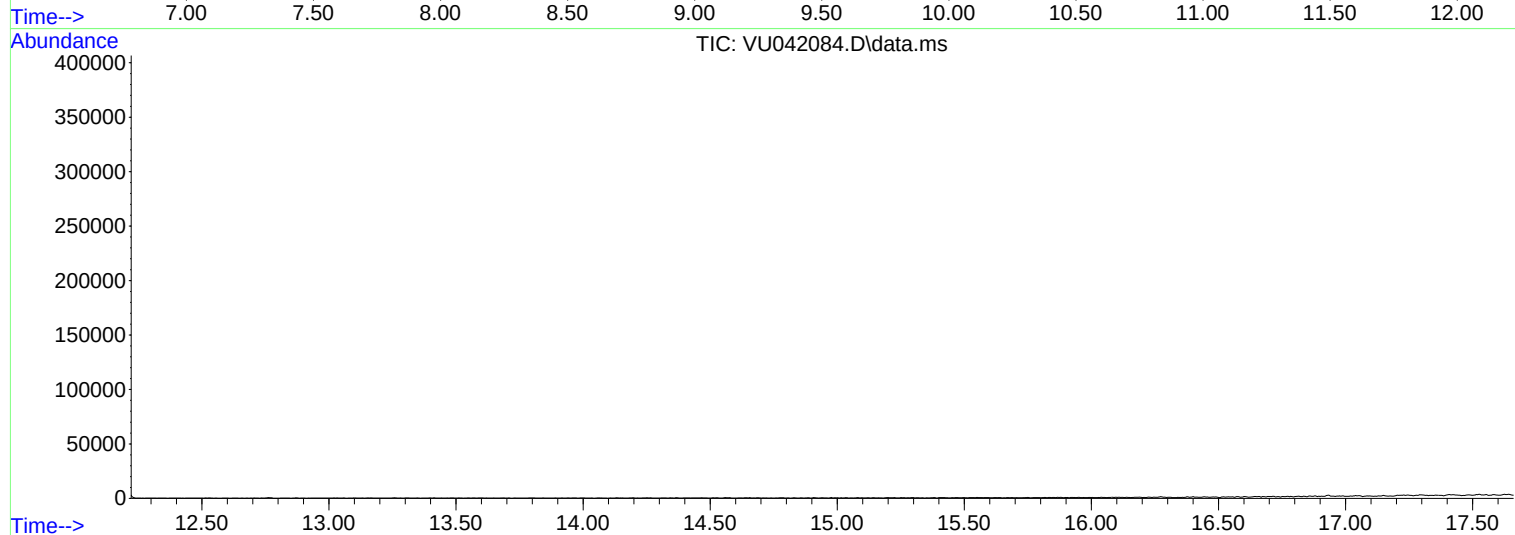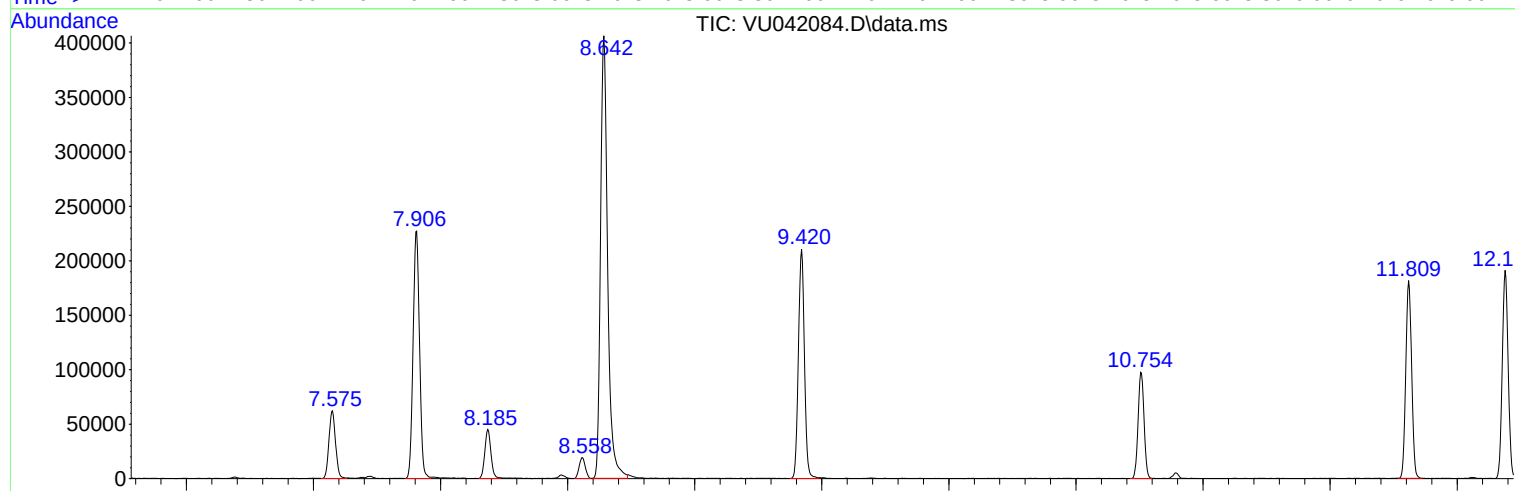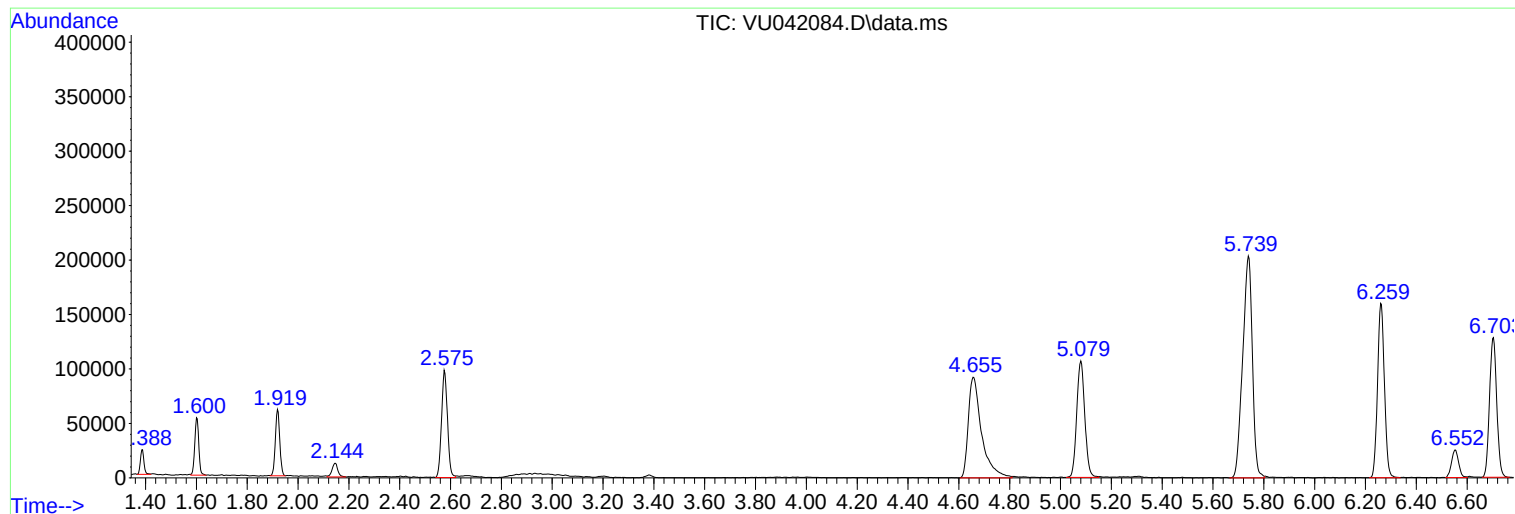

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
Data File : VU042084.D
Acq On : 15 Jan 2021 20:02
Operator : SY/MD
Sample : M1164-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXQ0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
Data File : VU042084.D
Acq On : 15 Jan 2021 20:02
Operator : SY/MD
Sample : M1164-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXQ0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
