
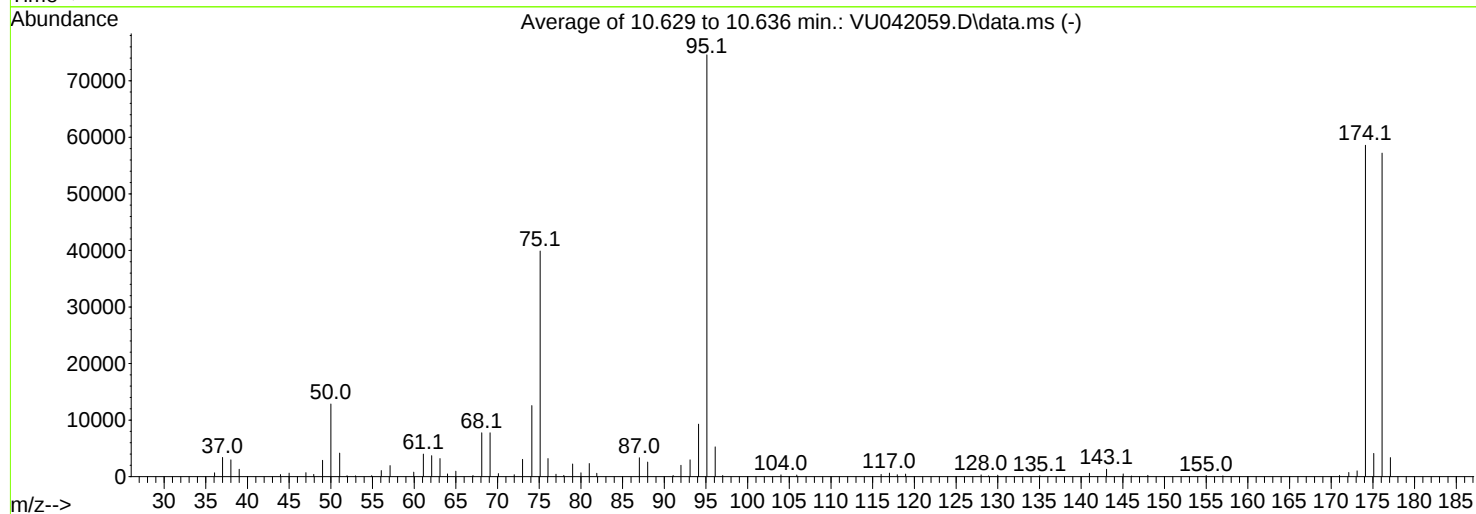


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011521\
Data File : VU042059.D
Acq On : 15 Jan 2021 09:09
Operator : SY/MD
Sample : BFB37
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB37

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR011321WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat Jan 16 01:05:16 2021

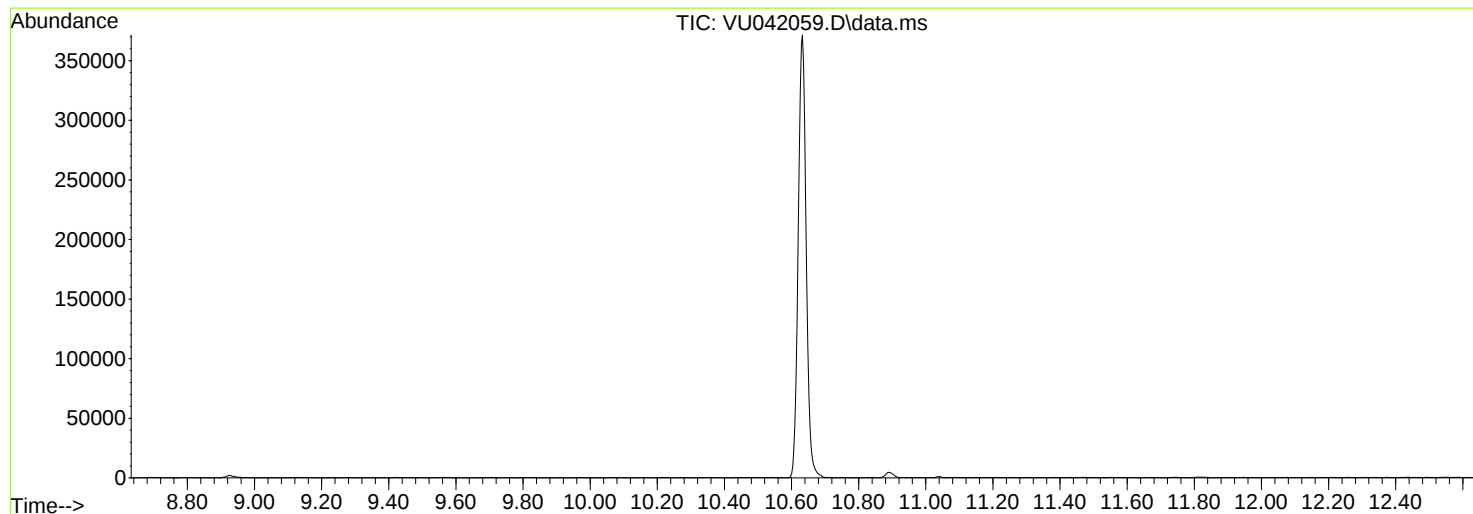

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.2	12843	PASS
75	95	30	80	53.5	39891	PASS
95	95	100	100	100.0	74579	PASS
96	95	5	9	7.1	5267	PASS
173	174	0.00	2	1.7	1023	PASS
174	95	50	120	78.6	58600	PASS
175	174	5	9	7.0	4114	PASS
176	174	95	101	97.6	57197	PASS
177	176	5	9	5.9	3372	PASS

m/z	Abundance
43.90	198.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37

m/z	Abundance
36.10	680.0
37.00	3693.0
38.00	2863.0
39.00	1395.0
44.00	622.0
45.00	631.0
47.00	729.0
48.00	449.0
49.00	2787.0
50.00	13178.0
51.10	4102.0
52.00	109.0
52.90	136.0
54.90	193.0
56.00	1163.0
57.10	2062.0
60.00	762.0
61.10	4258.0
62.10	3868.0
63.10	3320.0
64.00	457.0
65.00	983.0
67.00	183.0
68.10	7554.0
69.10	7913.0
70.10	462.0
72.00	349.0
73.00	3052.0
74.10	12445.0
75.10	40920.0
76.10	3205.0
77.00	431.0
77.90	253.0
79.00	2352.0
80.00	796.0
81.00	2389.0
81.90	609.0
87.00	3264.0
88.00	2615.0
91.10	150.0
92.00	1962.0
93.10	2921.0
94.10	9644.0
95.10	75440.0
96.10	5234.0
97.00	206.0
104.00	293.0
105.00	123.0
105.90	316.0
116.00	448.0
117.00	688.0
117.90	372.0
118.90	415.0
128.00	329.0
128.90	110.0
130.00	244.0
131.10	101.0
135.00	160.0
141.00	672.0
143.10	1298.0
145.10	553.0
146.10	126.0
148.00	231.0
155.00	198.0
157.00	145.0
171.00	179.0
172.10	662.0
173.10	896.0
174.10	58424.0
175.10	4208.0
176.10	56064.0
177.10	3464.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37

m/z	Abundance
36.10	708.0
37.00	3479.0
38.00	3071.0
39.00	1321.0
44.00	602.0
45.00	666.0
47.00	726.0
47.90	415.0
49.00	2967.0
50.00	13121.0
51.00	4262.0
51.90	170.0
52.90	166.0
54.90	174.0
56.10	1080.0
57.10	2016.0
60.00	825.0
61.10	4112.0
62.10	3799.0
63.10	3303.0
64.00	522.0
65.00	1001.0
67.00	196.0
68.10	8105.0
69.10	7845.0
70.10	571.0
72.00	349.0
73.00	3148.0
74.10	12943.0
75.10	41032.0
76.00	3289.0
77.00	406.0
78.00	239.0
79.00	2280.0
80.00	679.0
81.00	2346.0
81.90	614.0
87.00	3447.0
88.00	2659.0
91.10	201.0
92.00	2071.0
93.10	2969.0
94.10	9580.0
95.10	76584.0
96.10	5441.0
97.00	236.0
104.00	333.0
105.90	295.0
116.00	430.0
117.00	616.0
117.90	376.0
119.00	466.0
128.00	328.0
128.90	147.0
130.00	290.0
135.10	179.0
141.00	608.0
143.10	1346.0
145.10	490.0
146.00	134.0
148.00	263.0
155.00	199.0
157.00	161.0
171.00	186.0
172.10	737.0
173.10	1045.0
174.10	60376.0
175.10	4216.0
176.10	59096.0
177.10	3482.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37

m/z	Abundance
36.00	669.0
37.00	3009.0
38.00	2993.0
39.00	1189.0
44.00	464.0
45.00	565.0
47.00	682.0
47.90	369.0
49.00	2886.0
50.00	12231.0
51.00	4093.0
51.90	215.0
53.00	148.0
54.90	136.0
56.10	989.0
57.10	1781.0
59.90	796.0
61.10	3559.0
62.10	3495.0
63.10	2958.0
64.00	502.0
65.00	936.0
67.10	190.0
68.10	7578.0
69.10	7474.0
70.10	617.0
72.00	292.0
73.00	2933.0
74.10	12258.0
75.10	37720.0
76.00	3104.0
77.00	398.0
78.00	231.0
79.00	2069.0
80.00	557.0
81.00	2210.0
81.90	603.0
87.00	3319.0
88.00	2436.0
91.00	253.0
92.00	1958.0
93.10	3006.0
94.10	8583.0
95.10	71712.0
96.10	5125.0
97.00	182.0
104.00	316.0
105.90	272.0
116.00	334.0
117.00	539.0
118.00	273.0
119.00	464.0
128.00	256.0
128.90	163.0
130.00	277.0
135.10	181.0
141.00	551.0
143.00	1268.0
145.00	403.0
146.00	125.0
148.00	232.0
155.00	208.0
157.00	143.0
171.00	219.0
172.10	797.0
173.10	1128.0
174.10	57000.0
175.10	3918.0
176.10	56432.0
177.10	3169.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37