


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011524\
Data File : VU057516.D
Acq On : 15 Jan 2024 08:36
Operator : MD/SY
Sample : BFB107
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB107

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011124WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Jan 17 05:27:39 2024

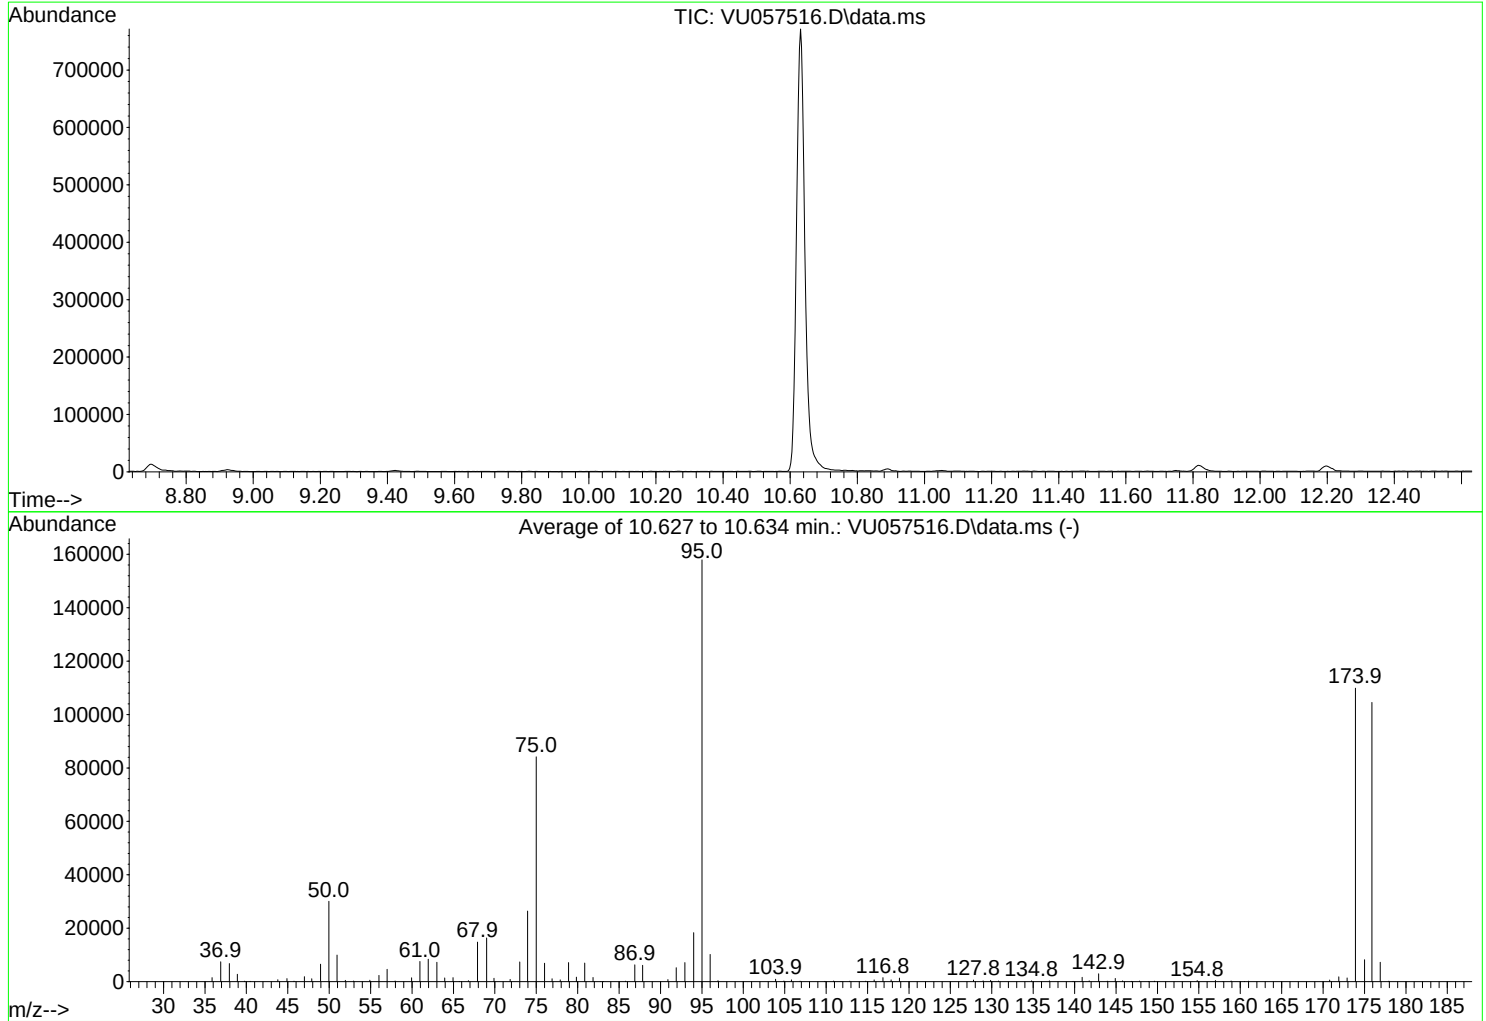

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	30059	PASS
75	95	30	80	53.3	84171	PASS
95	95	100	100	100.0	157931	PASS
96	95	5	9	6.5	10207	PASS
173	174	0.00	2	1.3	1389	PASS
174	95	50	120	69.6	109883	PASS
175	174	5	9	7.5	8213	PASS
176	174	95	101	95.1	104536	PASS
177	176	5	9	6.9	7233	PASS

m/z	Abundance
35.80	229.0
39.90	183.0
43.80	418.0

Instrument :
MSVOA_U
ClientSampleId :
BFB107

m/z	Abundance
35.90	1696.0
36.90	7403.0
37.90	6753.0
38.90	2844.0
39.80	329.0
40.50	172.0
43.80	1161.0
44.90	1182.0
45.70	171.0
47.00	1679.0
47.90	1084.0
48.90	6425.0
50.00	29744.0
51.00	10253.0
51.90	441.0
52.90	243.0
54.90	557.0
56.00	2417.0
57.00	4566.0
57.90	200.0
60.00	1445.0
61.00	7736.0
62.00	8374.0
63.00	7258.0
64.00	1351.0
64.90	1530.0
65.70	120.0
66.80	367.0
67.90	14428.0
69.00	16239.0
69.90	1444.0
71.80	813.0
73.00	7662.0
74.00	26520.0
75.00	83512.0
76.00	7164.0
76.80	1084.0
77.90	658.0
78.90	7170.0
79.80	1698.0
80.80	6865.0
81.90	1545.0
82.80	103.0
85.80	191.0
86.90	5834.0
87.90	5988.0
90.90	696.0
91.90	5228.0
93.00	7419.0
94.00	18120.0
95.00	153216.0
96.00	10262.0
97.00	389.0
103.90	935.0
105.00	234.0
105.80	713.0
106.90	213.0
109.90	120.0
110.90	200.0
112.80	138.0
114.80	182.0
115.70	731.0
116.80	1487.0
117.90	567.0
118.80	1279.0
127.80	620.0
129.00	262.0
129.80	487.0
130.80	220.0
134.80	323.0
136.90	279.0
140.90	1489.0
141.80	249.0
142.90	2955.0
144.00	218.0
144.90	1187.0
145.80	341.0
146.90	181.0
147.90	230.0
148.90	114.0
149.70	199.0
154.80	291.0
157.00	391.0
158.90	216.0
160.50	118.0
161.10	139.0
170.80	602.0
171.90	1788.0
172.90	1392.0
173.90	106560.0
175.00	8296.0
175.90	101456.0

Instrument :
MSVOA_U
ClientSampleId :
BFB107

176.907056.0

178.00146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB107

m/z	Abundance
35.90	1756.0
36.90	7634.0
38.00	7048.0
38.90	2873.0
39.70	324.0
43.80	1192.0
44.90	1142.0
45.70	223.0
47.00	1943.0
47.90	1188.0
49.00	6717.0
49.90	30976.0
51.00	10257.0
51.90	515.0
53.00	262.0
54.90	538.0
56.00	2415.0
57.00	4704.0
57.90	240.0
60.00	1455.0
60.90	7792.0
62.00	8682.0
63.00	7428.0
64.00	1404.0
65.00	1526.0
65.90	107.0
66.80	338.0
67.90	15231.0
69.00	16968.0
69.90	1270.0
71.80	814.0
73.00	7567.0
74.00	27160.0
75.00	86816.0
76.00	7127.0
76.90	1106.0
77.90	687.0
78.90	7375.0
79.80	1675.0
80.90	7144.0
81.80	1607.0
83.10	126.0
85.80	182.0
86.90	6435.0
87.90	6303.0
90.90	794.0
91.90	5378.0
93.00	7223.0
94.00	18800.0
95.00	163456.0
96.00	10457.0
97.00	390.0
103.90	976.0
104.90	257.0
105.80	653.0
106.90	219.0
109.80	125.0
110.90	235.0
112.80	166.0
114.80	198.0
115.80	698.0
116.90	1569.0
117.80	669.0
118.90	1350.0
127.80	629.0
129.00	294.0
129.90	496.0
130.80	247.0
134.80	307.0
136.90	288.0
139.80	144.0
140.90	1662.0
141.70	314.0
142.90	3022.0
143.90	198.0
144.90	1269.0
145.80	274.0
146.90	146.0
147.90	232.0
149.60	225.0
154.80	412.0
157.00	417.0
157.90	113.0
158.90	262.0
160.50	153.0
161.00	171.0
170.80	648.0
171.90	1895.0
172.90	1454.0
173.90	112744.0
175.00	8449.0
175.90	107272.0

Instrument :
MSVOA_U
ClientSampleId :
BFB107

176.907636.0

178.00173.0

Instrument :
MSVOA_U
ClientSampleId :
BFB107

m/z	Abundance
35.90	1662.0
36.90	7275.0
38.00	6611.0
38.90	2652.0
39.70	367.0
40.40	227.0
43.80	1144.0
44.90	1120.0
45.80	226.0
47.00	2030.0
47.90	1021.0
49.00	6476.0
49.90	29456.0
50.90	9391.0
52.00	493.0
53.00	277.0
54.90	480.0
56.00	2241.0
57.00	4522.0
58.00	266.0
59.90	1438.0
60.90	7179.0
61.90	8205.0
63.00	7062.0
63.90	1427.0
65.00	1527.0
66.00	145.0
66.80	354.0
67.90	14793.0
69.00	15829.0
69.90	1086.0
71.90	826.0
73.00	6846.0
73.90	25536.0
75.00	82184.0
76.00	6435.0
77.00	1110.0
77.90	599.0
78.90	6912.0
79.90	1710.0
80.90	6935.0
81.80	1534.0
83.10	151.0
85.80	179.0
86.90	6558.0
87.80	6056.0
90.90	792.0
91.90	4994.0
92.90	6681.0
94.00	18048.0
95.00	157120.0
96.00	9901.0
96.90	359.0
103.90	877.0
104.80	263.0
105.80	592.0
106.80	211.0
109.80	129.0
110.90	218.0
111.80	105.0
112.90	187.0
114.80	177.0
115.90	598.0
116.90	1538.0
117.80	695.0
118.90	1301.0
127.80	620.0
128.90	327.0
129.90	545.0
130.80	244.0
134.80	284.0
137.00	309.0
139.80	189.0
140.90	1681.0
141.70	279.0
142.90	2864.0
143.90	174.0
144.90	1217.0
145.80	212.0
146.80	125.0
147.80	226.0
149.60	194.0
154.80	517.0
157.00	398.0
157.90	151.0
158.90	240.0
160.90	223.0
170.80	586.0
171.90	1769.0
172.90	1321.0
173.90	110344.0
175.00	7895.0

Instrument :
MSVOA_U
ClientSampleId :
BFB107

175.90	104880.0
176.90	7008.0
177.90	240.0

Instrument :
MSVOA_U
ClientSampleId :
BFB107