

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011525\
 Data File : VU062763.D
 Acq On : 15 Jan 2025 13:37
 Operator : MD/SY
 Sample : Q1057-16 10X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH8W5

Quant Time: Jan 16 00:47:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 16 00:44:09 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.239	114	94628	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.406	117	91442	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	43598	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	16948	3.234	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	64.600%
7) Chloroethane-d5	1.901	69	16568	3.930	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.600%
11) 1,1-Dichloroethene-d2	2.554	65	9639	3.550	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.000%
20) 2-Butanone-d5	4.605	46	60044	56.056	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.120%
24) Chloroform-d	5.049	84	56939	4.416	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.400%
26) 1,2-Dichloroethane-d4	5.689	65	33140	4.738	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.800%
32) Benzene-d6	5.714	84	90753	4.060	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.200%
36) 1,2-Dichloropropane-d6	6.676	67	27164	4.383	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.600%
41) Toluene-d8	7.888	98	85970	3.948	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.000%
43) trans-1,3-Dichloroprop...	8.171	79	12206	3.951	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.000%
46) 2-Hexanone-d5	8.618	63	48055	49.459	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.920%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	26010	5.011	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.200%
66) 1,2-Dichlorobenzene-d4	12.184	152	34151	4.708	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.200%
Target Compounds					Qvalue	
22) cis-1,2-Dichloroethene	4.647	96	5891	0.860	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011525\
Data File : VU062763.D
Acq On : 15 Jan 2025 13:37
Operator : MD/SY
Sample : Q1057-16 10X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH8W5


Quant Time: Jan 16 00:47:07 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 16 00:44:09 2025
Response via : Initial Calibration

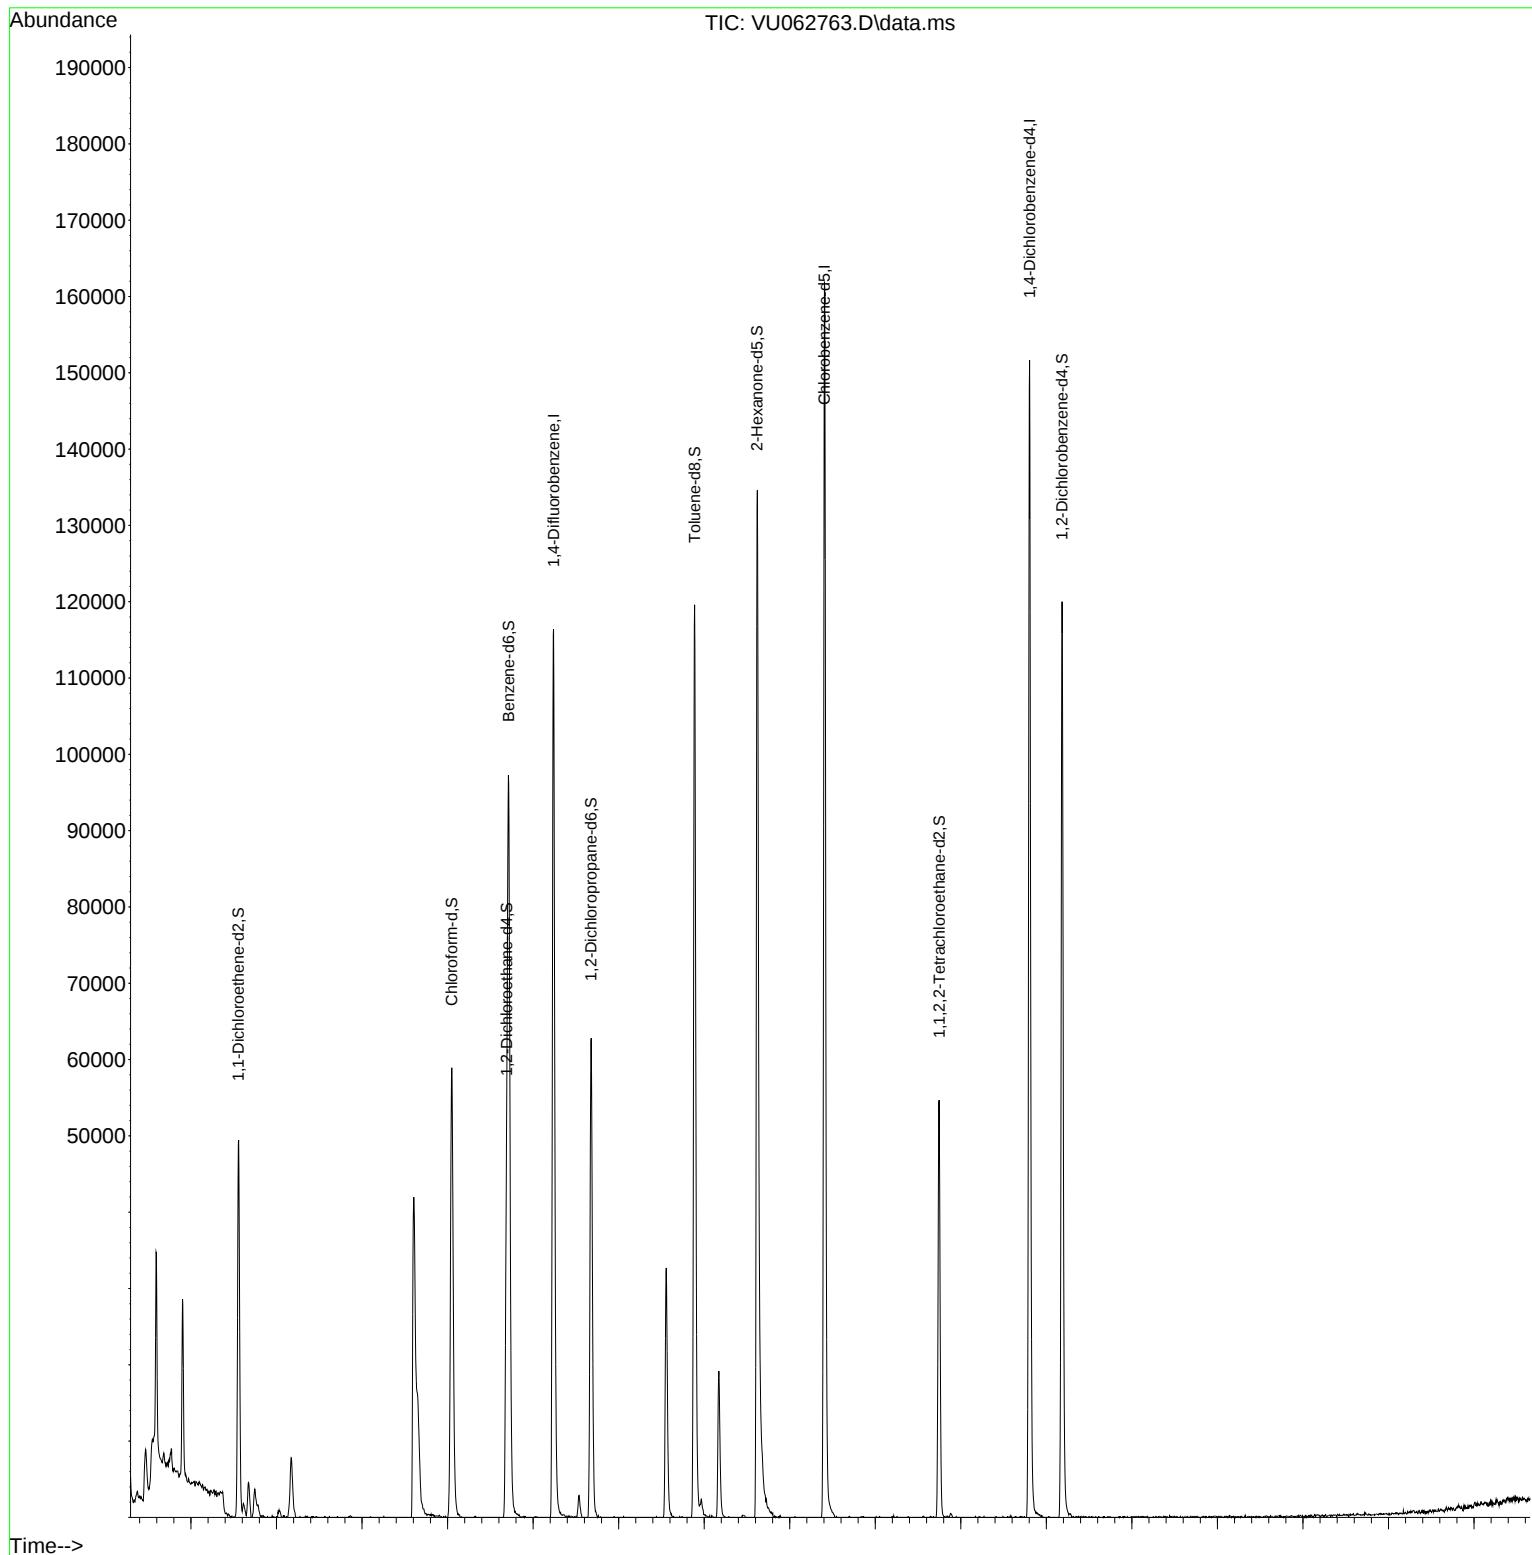

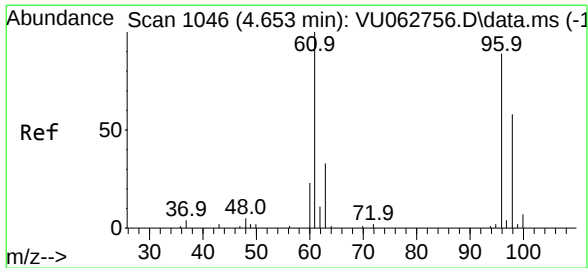

#22
 cis-1,2-Dichloroethene
 Concen: 0.860 ug/L
 RT: 4.647 min Scan# 10
 Delta R.T. -0.006 min
 Lab File: VU062763.D
 Acq: 15 Jan 2025 13:37

Instrument :
 MSVOA_U
 ClientSampleId :
 BH8W5

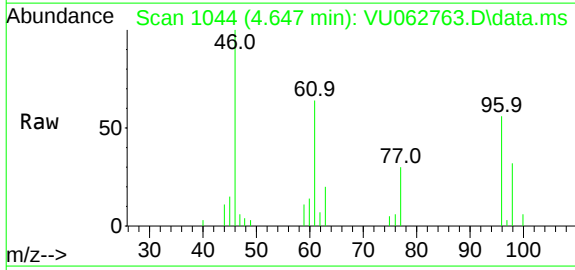

Tgt Ion:	96	Resp:	5891
Ion	Ratio	Lower	Upper
96	100		
61	115.4	84.8	157.6
98	58.3	43.1	80.1

