

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011525\
 Data File : VU062777.D
 Acq On : 15 Jan 2025 19:14
 Operator : MD/SY
 Sample : VIBLK197
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK197

Quant Time: Jan 16 00:51:54 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 16 00:44:09 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	84329	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	81786	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	39148	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	18151	3.886	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.800%
7) Chloroethane-d5	1.901	69	17570	4.677	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.600%
11) 1,1-Dichloroethene-d2	2.557	65	10514	4.345	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	87.000%
20) 2-Butanone-d5	4.608	46	45452	47.616	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.240%
24) Chloroform-d	5.049	84	60470	5.262	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.200%
26) 1,2-Dichloroethane-d4	5.689	65	36076	5.788	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	115.800%
32) Benzene-d6	5.714	84	99492	4.977	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.600%
36) 1,2-Dichloropropane-d6	6.679	67	29548	5.331	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.600%
41) Toluene-d8	7.888	98	91495	4.697	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.000%
43) trans-1,3-Dichloroprop...	8.171	79	13357	4.834	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.600%
46) 2-Hexanone-d5	8.621	63	42708	49.146	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.300%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	26515	5.712	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	114.200%
66) 1,2-Dichlorobenzene-d4	12.183	152	35985	5.525	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.600%
Target Compounds					Qvalue	
22) cis-1,2-Dichloroethene	4.660	96	2423	0.397	ug/L	# 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011525\
Data File : VU062777.D
Acq On : 15 Jan 2025 19:14
Operator : MD/SY
Sample : VIBLK197
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK197


Quant Time: Jan 16 00:51:54 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 16 00:44:09 2025
Response via : Initial Calibration

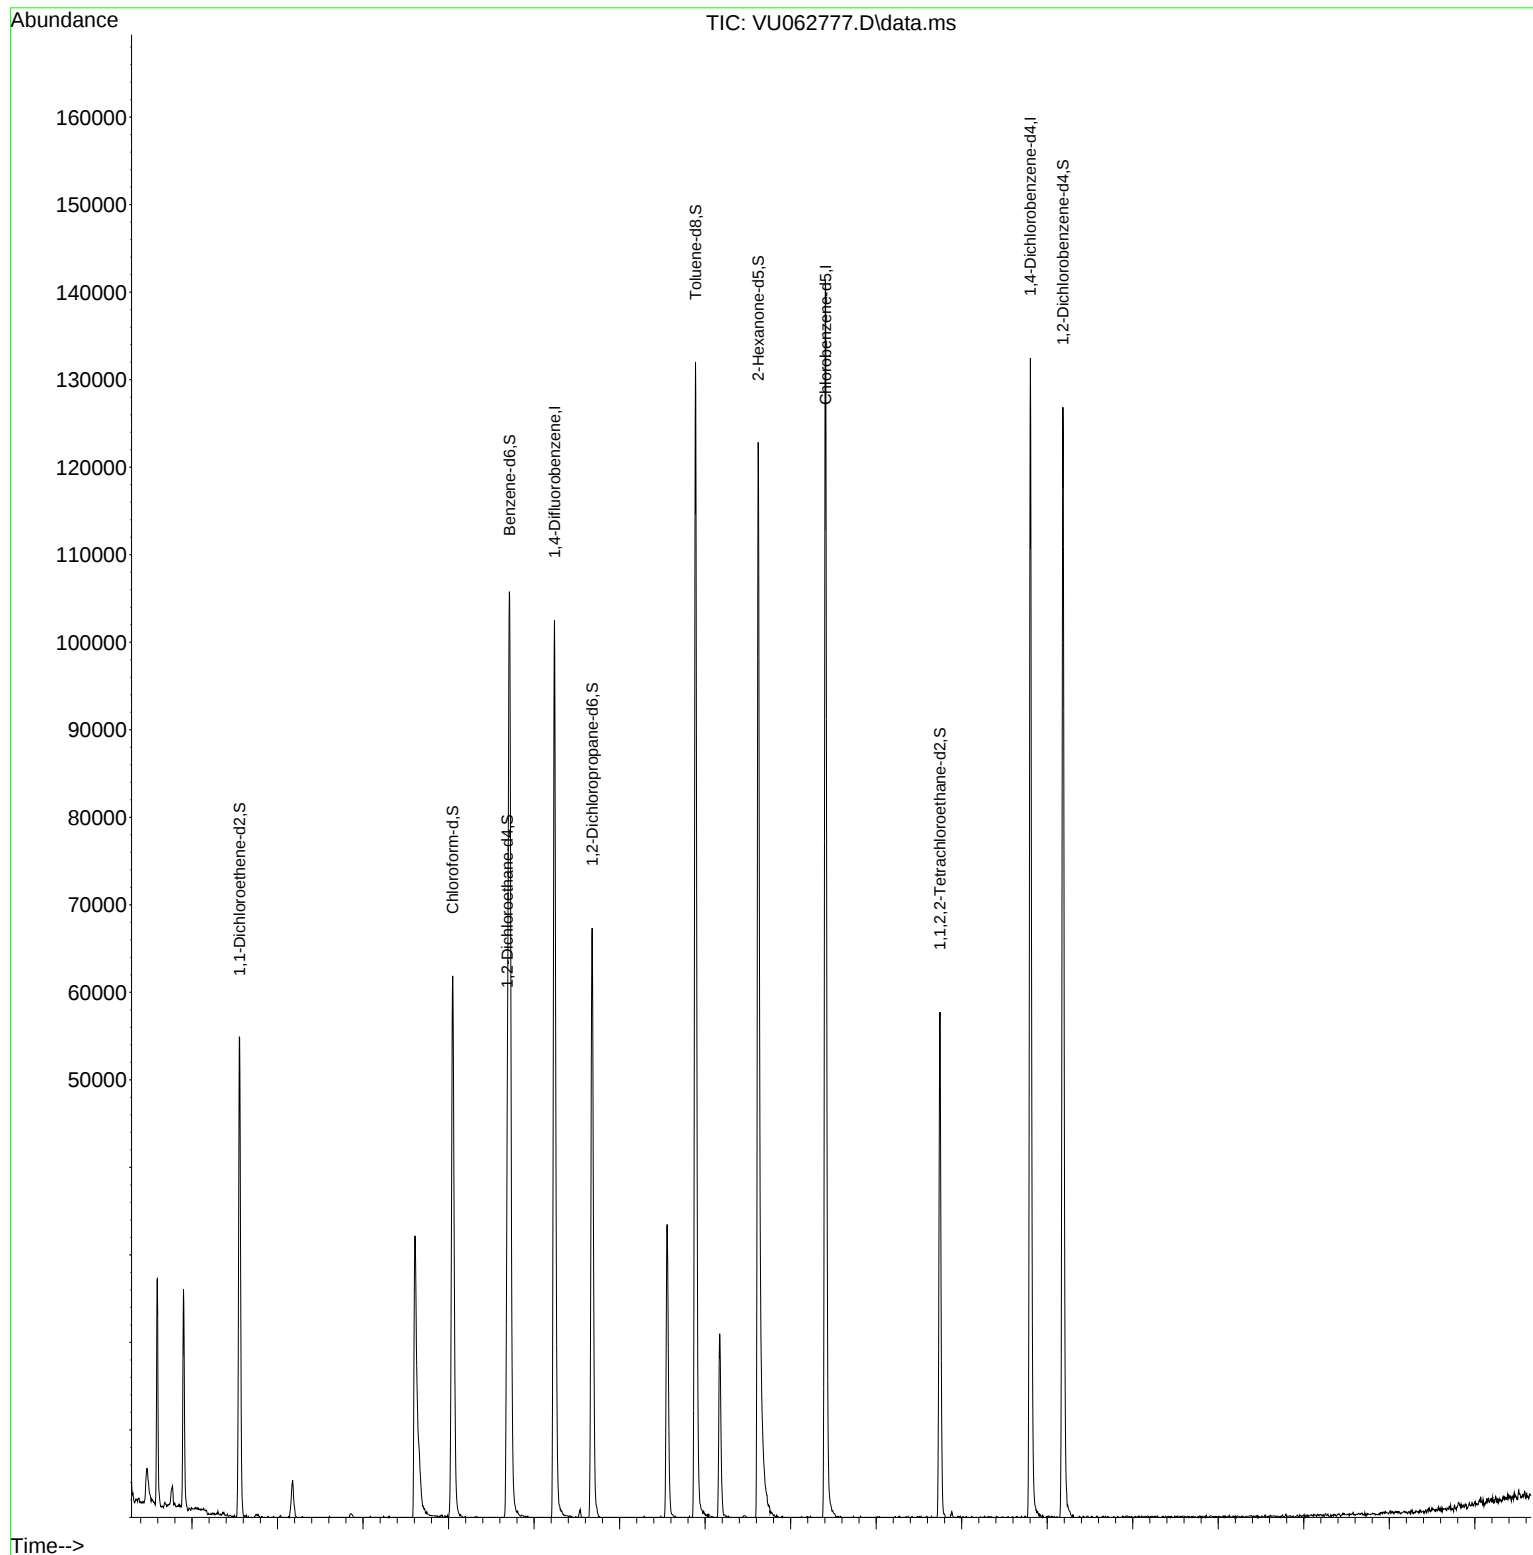

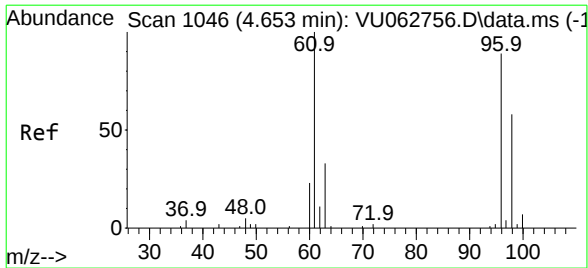

#22
 cis-1,2-Dichloroethene
 Concen: 0.397 ug/L
 RT: 4.660 min Scan# 10
 Delta R.T. 0.006 min
 Lab File: VU062777.D
 Acq: 15 Jan 2025 19:14

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK197

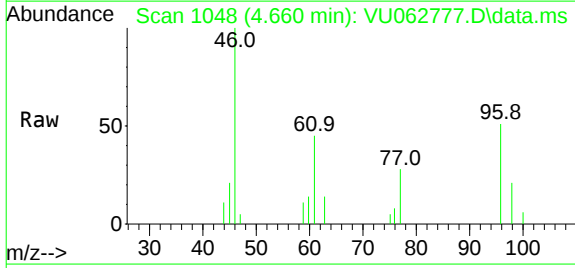

Tgt Ion:	96	Resp:	2423
Ion	Ratio	Lower	Upper
96	100		
61	88.9	84.8	157.6
98	40.4	43.1	80.1#

