

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011525\
 Data File : VU062783.D
 Acq On : 15 Jan 2025 22:46
 Operator : MD/SY
 Sample : Q1084-06
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BA5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU062783.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.467	47	55	71	rBV	13847	26107	9.12%	1.061%
2	1.595	87	95	107	rBV	22195	25245	8.82%	1.026%
3	1.766	139	148	155	rBV6	2009	3069	1.07%	0.125%
4	1.904	182	191	205	rVB	22823	29538	10.32%	1.200%
5	2.557	382	394	406	rBV	46363	77379	27.03%	3.144%
6	2.785	456	465	476	rBB2	2233	4051	1.42%	0.165%
7	3.168	574	584	586	rBV	3956	4926	1.72%	0.200%
8	4.605	1022	1031	1055	rBV	43614	106916	37.35%	4.344%
9	5.049	1153	1169	1187	rBV2	58397	132936	46.44%	5.401%
10	5.711	1357	1375	1405	rBV4	101078	273861	95.67%	11.127%
11	6.238	1527	1539	1566	rBV	114329	221651	77.43%	9.006%
12	6.679	1664	1676	1696	rBV2	66140	128685	44.95%	5.228%
13	7.557	1938	1949	1967	rBV	35903	63076	22.03%	2.563%
14	7.888	2040	2052	2077	rBV	123845	218487	76.32%	8.877%
15	8.171	2131	2140	2158	rBV	22317	37879	13.23%	1.539%
16	8.621	2270	2280	2322	rBV2	136095	286260	100.00%	11.631%
17	9.409	2513	2525	2551	rBV	159030	273905	95.68%	11.129%
18	10.746	2930	2941	2958	rBV	58457	95504	33.36%	3.880%
19	11.804	3259	3270	3300	rBV	141716	242202	84.61%	9.841%
20	12.183	3377	3388	3409	rBV	120350	209581	73.21%	8.515%




Sum of corrected areas: 2461258

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011525\
Data File : VU062783.D
Acq On : 15 Jan 2025 22:46
Operator : MD/SY
Sample : Q1084-06
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

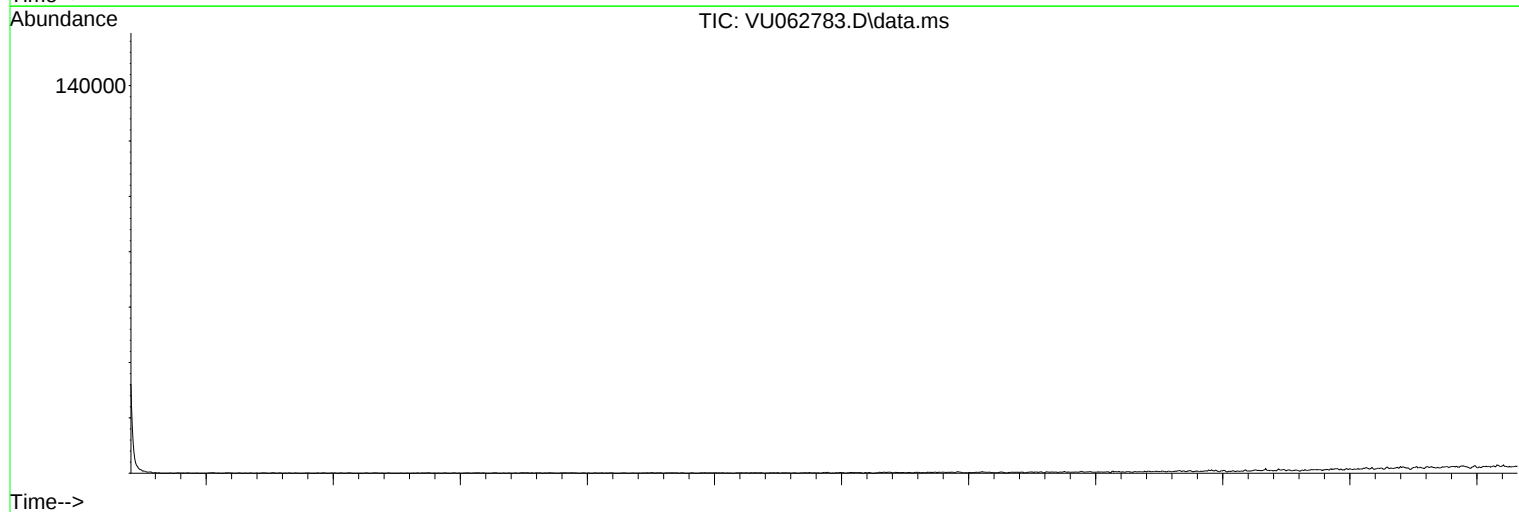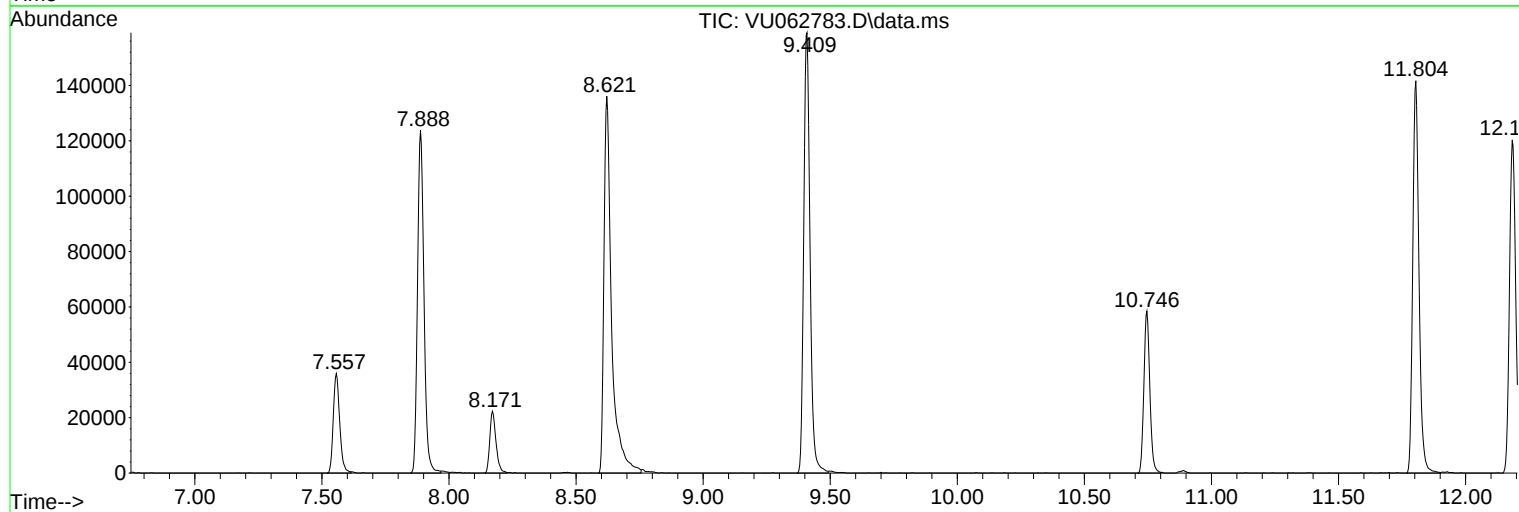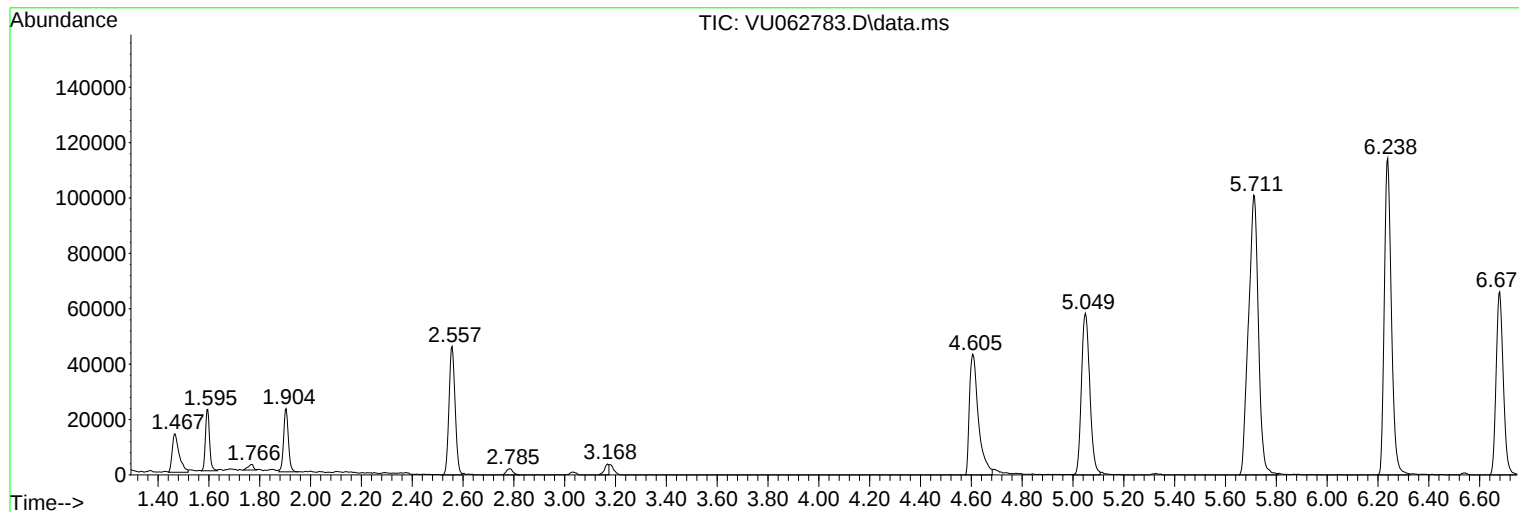

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011525\
Data File : VU062783.D
Acq On : 15 Jan 2025 22:46
Operator : MD/SY
Sample : Q1084-06
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011525\
Data File : VU062783.D
Acq On : 15 Jan 2025 22:46
Operator : MD/SY
Sample : Q1084-06
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc