

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU011619\
 Data File : VU029202.D
 Acq On : 16 Jan 2019 12:16
 Operator : JC/SP
 Sample : K1147-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TP-4

Quant Time: Jan 17 00:57:54 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jan 12 01:33:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.98	168	107748	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.88	114	189362	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	177592	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.48	152	70234	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	5.31	65	75173	56.44	ug/l	0.00
Spiked Amount			Recovery	=	112.88%	
35) Dibromofluoromethane	4.88	113	64532	52.57	ug/l	0.00
Spiked Amount			Recovery	=	105.14%	
50) Toluene-d8	7.56	98	247437	51.06	ug/l	0.00
Spiked Amount			Recovery	=	102.12%	
62) 4-Bromofluorobenzene	10.30	95	75931	43.60	ug/l	0.00
Spiked Amount			Recovery	=	87.20%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.33	50	540	Below Cal	#	79
5) Bromomethane	1.56	94	42	Below Cal	#	2
8) Diethyl Ether	2.10	74	907	1.100	ug/l	67
11) Tert butyl alcohol	2.83	59	184	0.543	ug/l #	73
14) Allyl chloride	2.70	41	1175	0.573	ug/l #	29
16) Acetone	2.32	43	7361	8.773	ug/l	96
17) Carbon Disulfide	2.48	76	250	Below Cal	#	75
18) Methyl Acetate	2.62	43	1099	0.563	ug/l #	51
20) Methylene Chloride	2.70	84	33417	23.456	ug/l	97
25) 2-Butanone	4.29	43	1339	1.181	ug/l	90
29) Tetrahydrofuran	4.66	42	547	0.796	ug/l #	30
31) Cyclohexane	4.98	56	1789	Below Cal	#	1
36) 1,1-Dichloropropene	4.98	75	7710	4.073	ug/l #	46
38) Carbon Tetrachloride	4.98	117	9827	6.225	ug/l #	18
41) Methacrylonitrile	4.66	41	228	0.205	ug/l #	21
43) Isopropyl Acetate	5.55	43	6851	2.150	ug/l #	93
45) 1,2-Dichloropropane	6.70	63	515	0.330	ug/l #	43
48) Methyl methacrylate	6.70	41	39278	25.310	ug/l #	37
51) 4-Methyl-2-Pentanone	7.42	43	34992	16.133	ug/l #	44
52) Toluene	7.64	92	3066	0.853	ug/l	85
54) cis-1,3-Dichloropropene	7.42	75	17623	7.398	ug/l #	62
57) 1,3-Dichloropropane	8.41	76	3543	1.438	ug/l #	42
59) 2-Hexanone	8.31	43	5522	3.243	ug/l #	21
76) 1,2,3-Trichloropropane	10.30	75	36925	21.458	ug/l #	36
80) 1,3,5-Trimethylbenzene	10.77	105	1350	0.311	ug/l	88
81) trans-1,4-Dichloro-2-buten	10.30	75	36925	55.340	ug/l #	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU011619\
Data File : VU029202.D
Acq On : 16 Jan 2019 12:16
Operator : JC/SP
Sample : K1147-12
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TP-4

Quant Time: Jan 17 00:57:54 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
Quant Title : SW846 8260
QLast Update : Sat Jan 12 01:33:59 2019
Response via : Initial Calibration

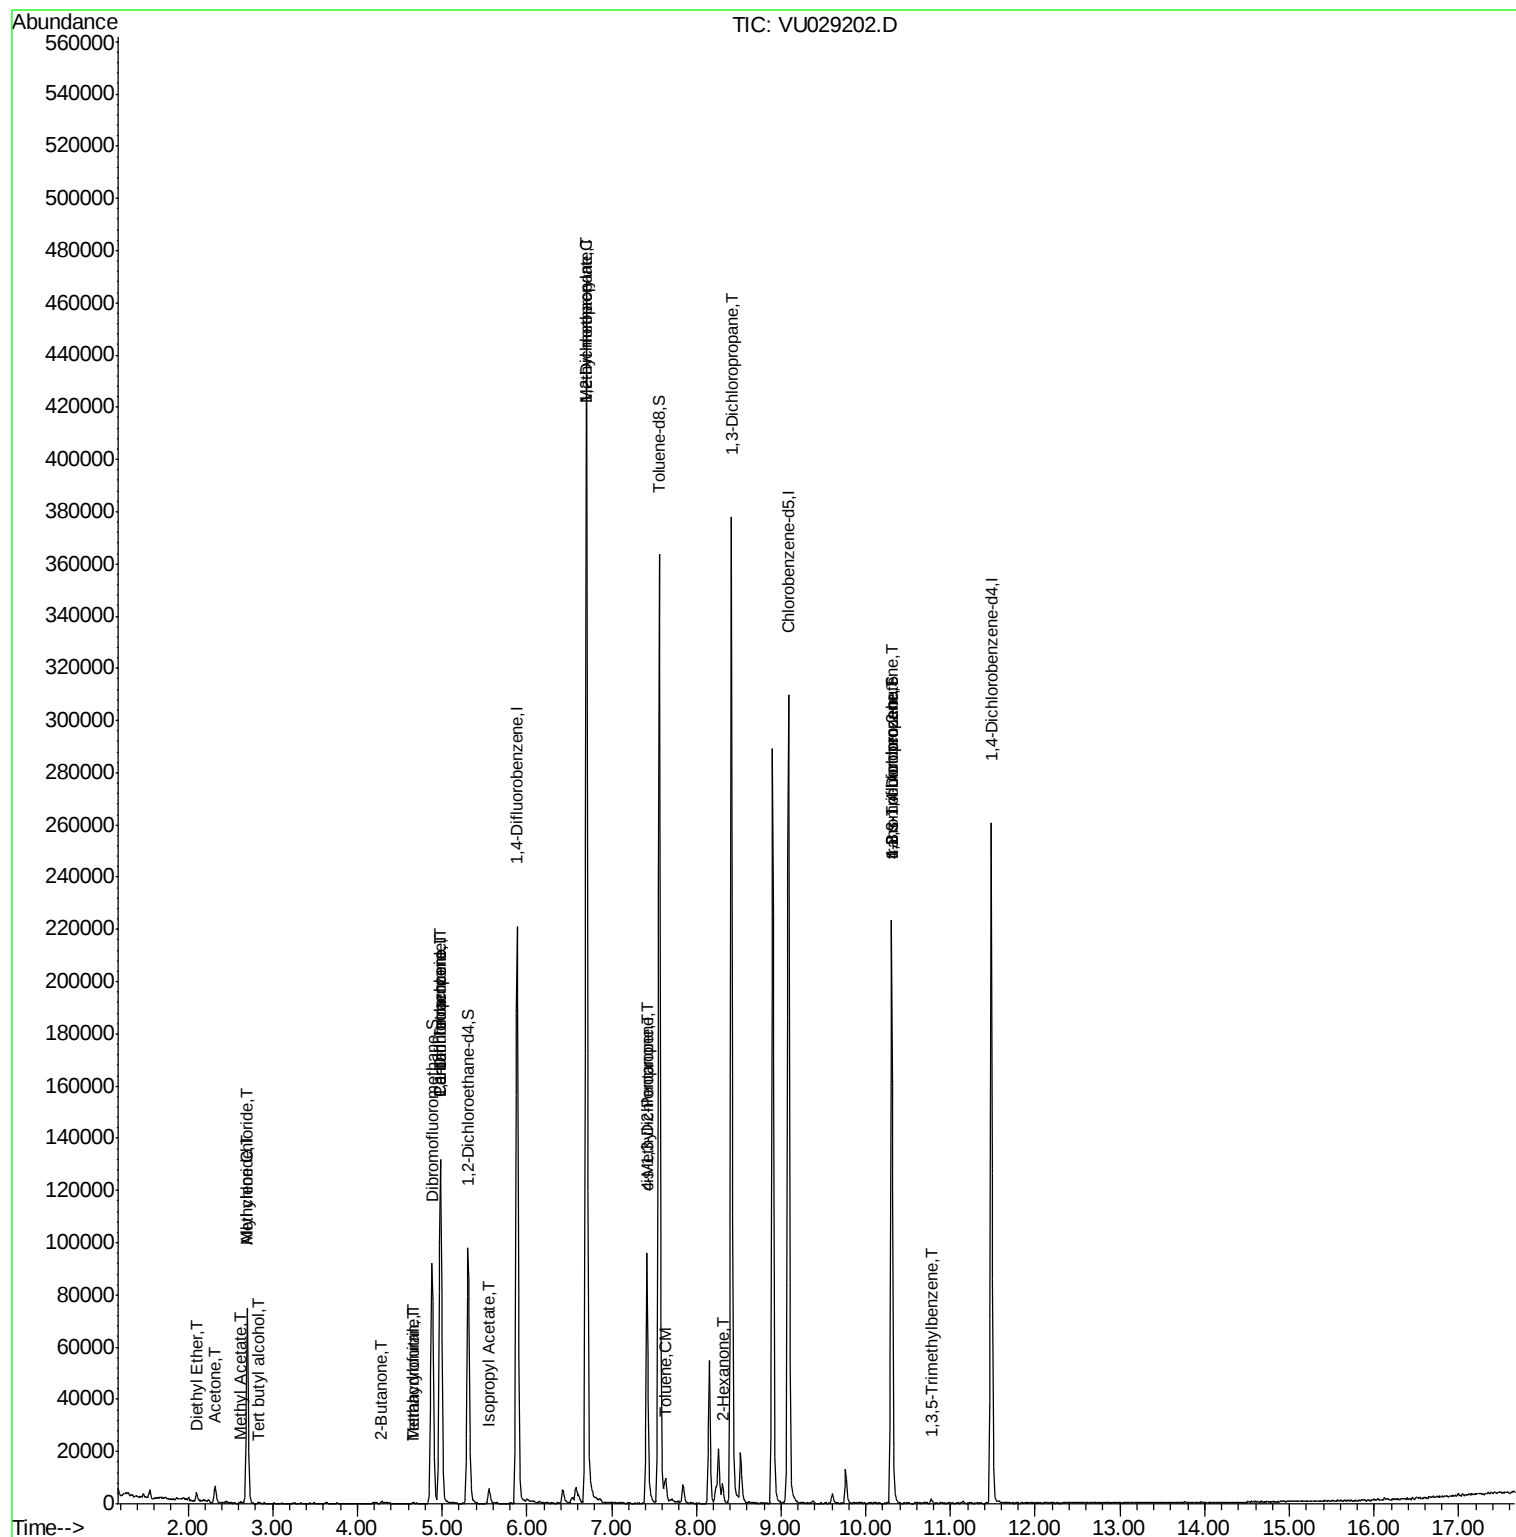

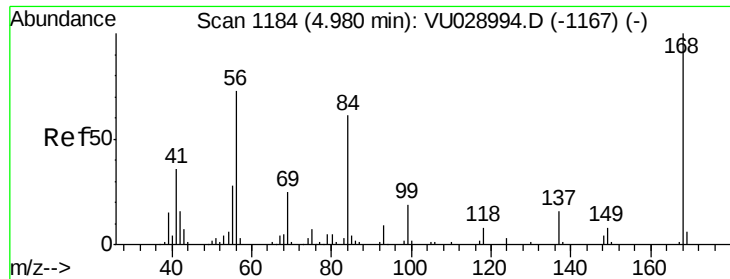

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.98 min Scan# 1184

Delta R.T. 0.00 min

Lab File: VU029202.D

Acq: 16 Jan 2019 12:16


Instrument :
MSVOA_U
ClientSampleId :
TP-4

Tot Ion:168 Resp: 107748

Ion Ratio Lower Upper

168 100

99 51.6 42.0 63.0

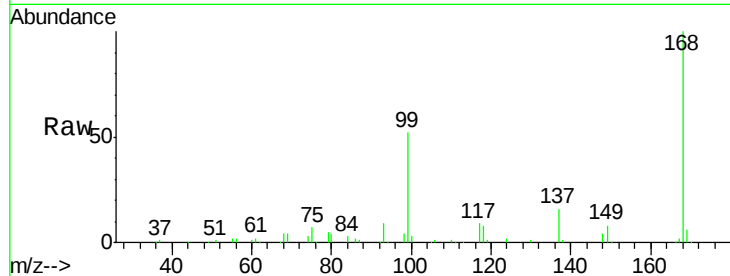

Abundance Ion 167.90 (167.60 to 168.60): VU028994.D (-1167) (-)

Ion 98.90 (98.60 to 99.60): VU028994.D (-1167) (-)

4.98

50000

40000

30000

20000

10000



0

4.90

5.00

5.10

Time-->

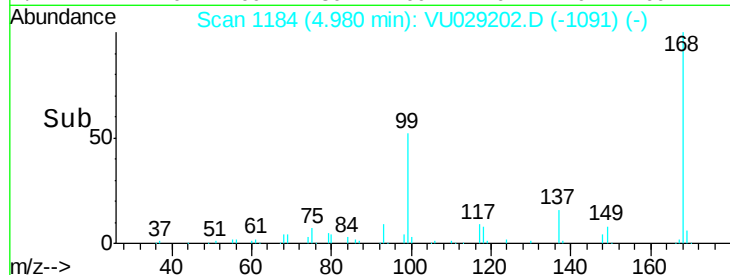

#3

Chloromethane

Concen: Below Cal

RT: 1.33 min Scan# 48

Delta R.T. 0.00 min

Lab File: VU029202.D


Acq: 16 Jan 2019 12:16

Tgt Ion: 50 Resp: 540

Ion Ratio Lower Upper

50 100

52 44.6 26.1 39.1#



Abundance Ion 49.90 (49.60 to 50.60): VU028994.D (-39) (-)

Ion 51.90 (51.60 to 52.60): VU028994.D (-39) (-)

1.33

600

500

400

300

200

100

0


1.30


1.32

1.34

1.36

Time-->

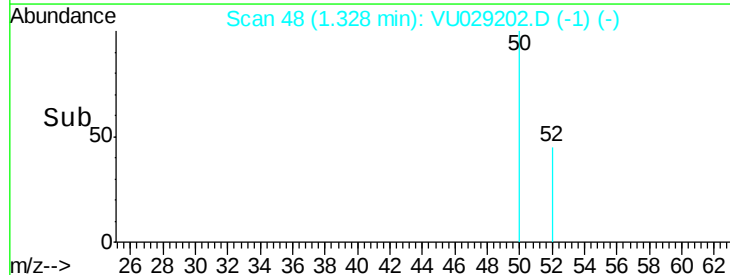



#5

Bromomethane

Concen: Below Cal

RT: 1.56 min Scan# 121

Delta R.T. -0.04 min

Lab File: VU029202.D

Acq: 16 Jan 2019 12:16

Instrument :

MSVOA_U

ClientSampled :


TP-4

Tot Ion: 94 Resp: 42

Ion Ratio Lower Upper

94 100

96 0.0 75.5 113.3#

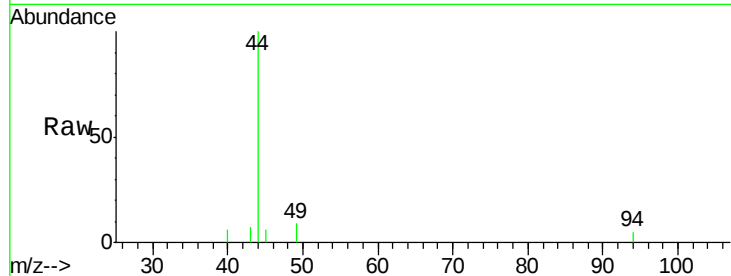

Abundance Ion 93.90 (93.60 to 94.60): VU0

Ion 95.90 (95.60 to 96.60): VU0

1.56

100

80



60

40

20

0

Time-->



#8

Diethyl Ether

Concen: 1.100 ug/l

RT: 2.10 min Scan# 289

Delta R.T. 0.00 min

Lab File: VU029202.D


Acq: 16 Jan 2019 12:16

Tgt Ion: 74 Resp: 907

Ion Ratio Lower Upper

74 100

45 125.4 46.9 140.6



Abundance Ion 74.00 (73.70 to 74.70): VU0

Ion 45.00 (44.70 to 45.70): VU0

2.10

800


600


400

200

0

Time-->









#11

Tert butyl alcohol
 Concen: 0.543 ug/l
 RT: 2.83 min Scan# 515
 Delta R.T. -0.00 min
 Lab File: VU029202.D
 Acq: 16 Jan 2019 12:16

Instrument :
 MSVOA_U
 ClientSampleId :
 TP-4




Tot Ion: 59 Resp: 184
 Ion Ratio Lower Upper
 59 100
 57 0.0 7.9 11.9#

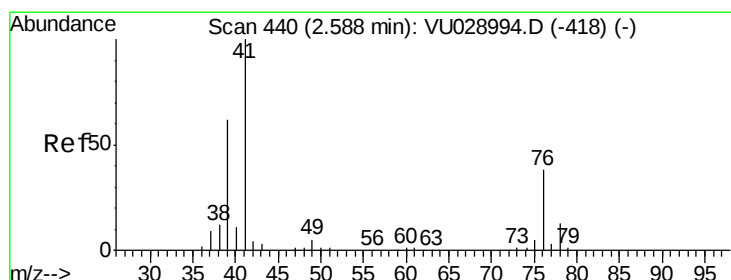


#14

Allyl chloride
 Concen: 0.573 ug/l
 RT: 2.70 min Scan# 474
 Delta R.T. 0.11 min
 Lab File: VU029202.D
 Acq: 16 Jan 2019 12:16

Tgt Ion: 41 Resp: 1175
 Ion Ratio Lower Upper
 41 100
 39 0.0 45.0 67.6#
 76 0.0 28.1 42.1#





#16

Acetone

Concen: 8.773 ug/l

RT: 2.32 min Scan# 357

Delta R.T. 0.00 min

Lab File: VU029202.D

Acq: 16 Jan 2019 12:16

Instrument :

MSVOA_U

ClientSampleId :





TP-4

Tot Ion: 43 Resp: 7361

Ion Ratio Lower Upper

43 100

58 33.3 28.6 42.8

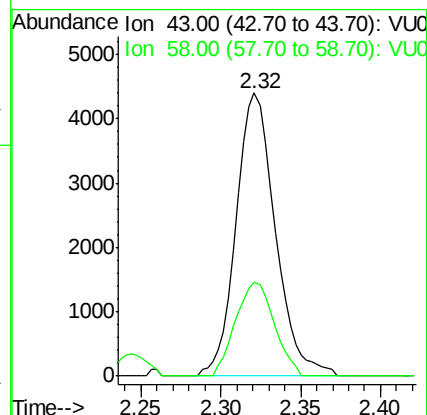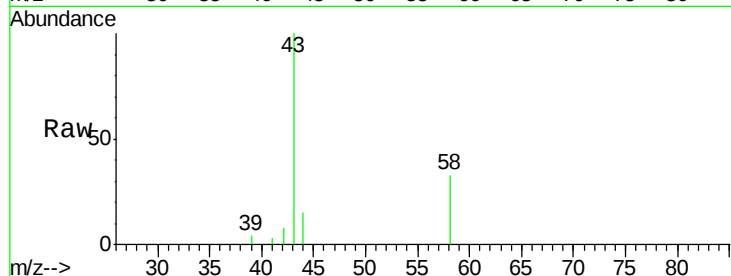

#17

Carbon Disulfide

Concen: Below Cal

RT: 2.48 min Scan# 405

Delta R.T. 0.00 min

Lab File: VU029202.D




Acq: 16 Jan 2019 12:16


Tgt Ion: 76 Resp: 250

Ion Ratio Lower Upper

76 100

78 0.0 7.2 10.8#



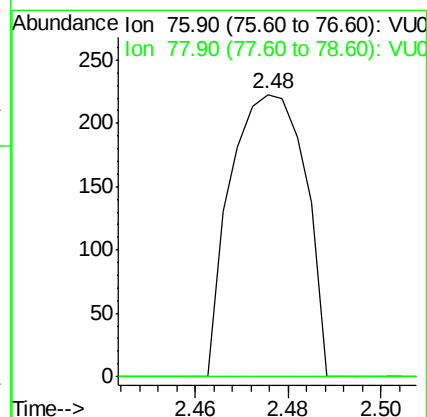





#18
Methyl Acetate
Concen: 0.563 ug/l
RT: 2.62 min Scan# 451
Delta R.T. 0.01 min
Lab File: VU029202.D
Acq: 16 Jan 2019 12:16




Instrument :
MSVOA_U
ClientSampleId :
TP-4


Tot Ion: 43 Resp: 1099
Ion Ratio Lower Upper
43 100
74 0.0 19.5 29.3#

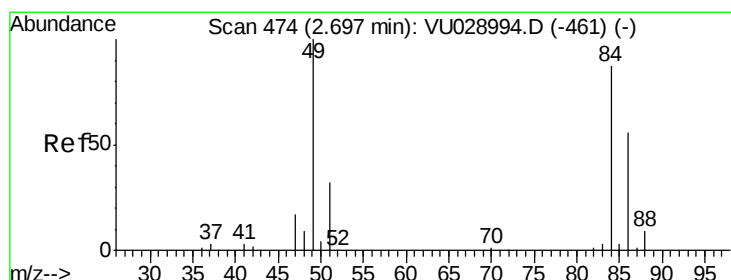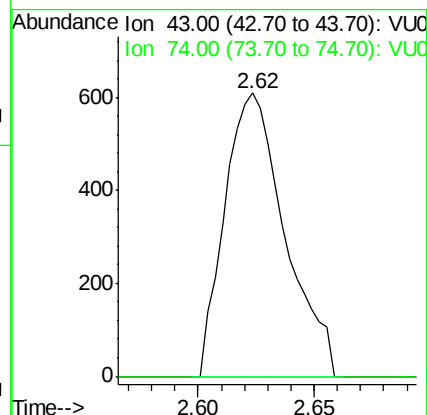

#20
Methylene Chloride
Concen: 23.456 ug/l
RT: 2.70 min Scan# 475
Delta R.T. 0.00 min
Lab File: VU029202.D
Acq: 16 Jan 2019 12:16

Tgt Ion: 84 Resp: 33417
Ion Ratio Lower Upper
84 100
49 119.0 91.9 137.9
51 38.2 29.2 43.8
86 64.1 51.8 77.6

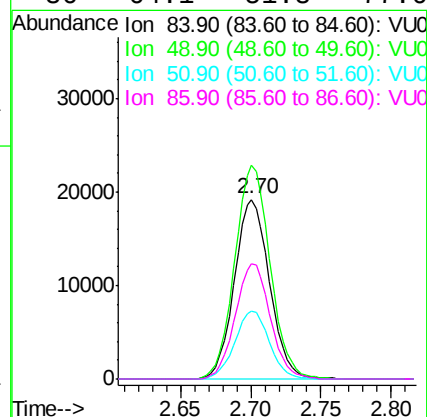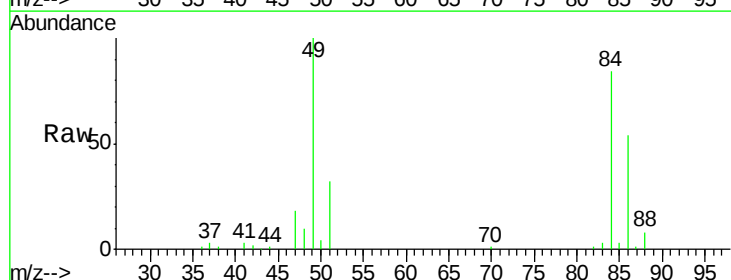

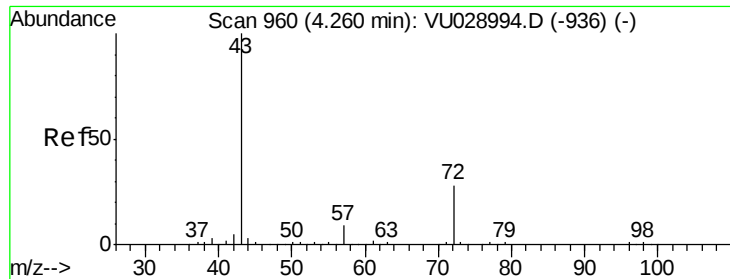

#25

2-Butanone

Concen: 1.181 ug/l

RT: 4.29 min Scan# 969

Delta R.T. 0.03 min

Lab File: VU029202.D

Acq: 16 Jan 2019 12:16





Instrument :
MSVOA_U
ClientSampleId :
TP-4

Tot Ion: 43 Resp: 1339

Ion Ratio Lower Upper

43 100

72 22.9 22.6 33.8

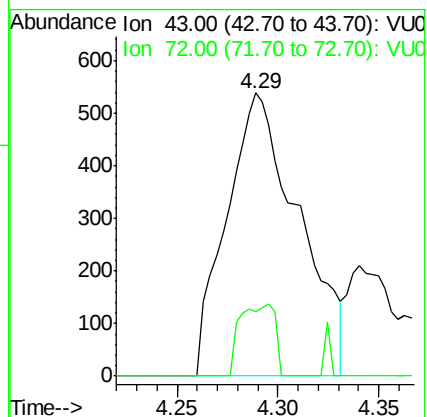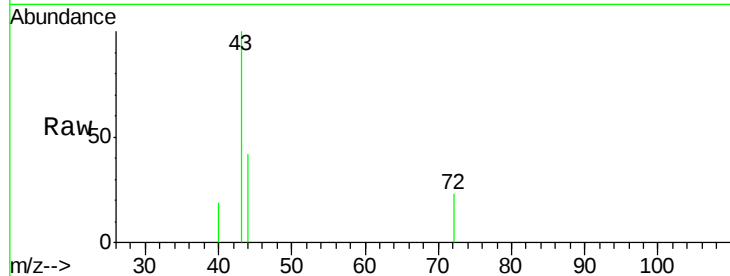

#29

Tetrahydrofuran

Concen: 0.796 ug/l

RT: 4.66 min Scan# 1085

Delta R.T. 0.03 min

Lab File: VU029202.D

Acq: 16 Jan 2019 12:16




Tgt Ion: 42 Resp: 547


Ion Ratio Lower Upper

42 100

72 0.0 38.3 57.5#

71 0.0 36.1 54.1#

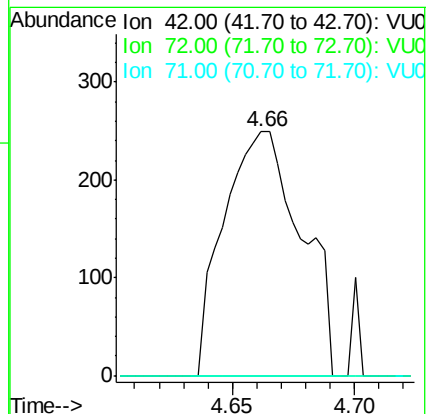

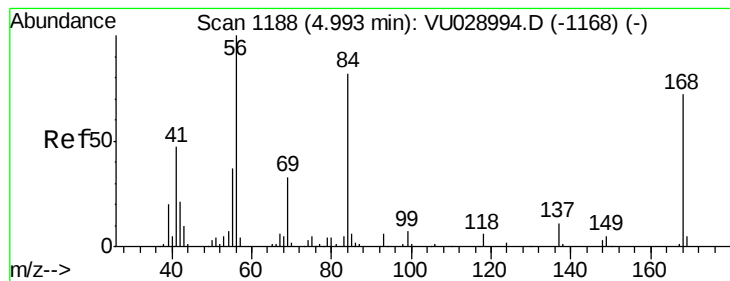

#31

Cyclohexane

Concen: Below Cal

RT: 4.98 min Scan# 1185

Delta R.T. -0.01 min

Lab File: VU029202.D

Acq: 16 Jan 2019 12:16

Instrument :

MSVOA_U

ClientSampleId :

TP-4


Tot Ion: 56 Resp: 1789

Ion Ratio Lower Upper

56 100

69 182.2 26.7 40.1#




84 176.5 65.7 98.5#



Abundance Ion 56.00 (55.70 to 56.70): VU028994.D (-1168) (-)

Ion 69.00 (68.70 to 69.70): VU028994.D (-1168) (-)

Ion 84.00 (83.70 to 84.70): VU028994.D (-1168) (-)

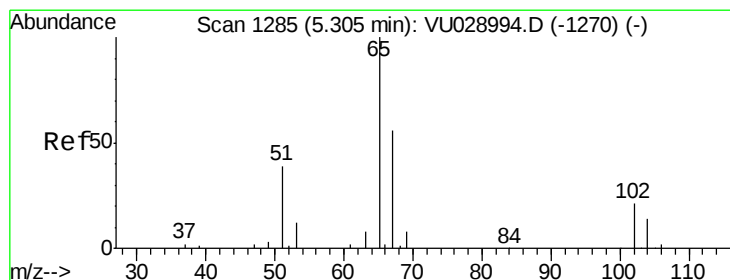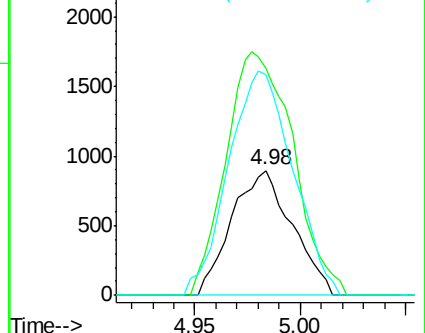

#33

1,2-Dichloroethane-d4

Concen: 56.437 ug/l

RT: 5.31 min Scan# 1286

Delta R.T. 0.00 min

Lab File: VU029202.D


Acq: 16 Jan 2019 12:16

Tgt Ion: 65 Resp: 75173

Ion Ratio Lower Upper



65 100


67 54.7 0.0 111.0

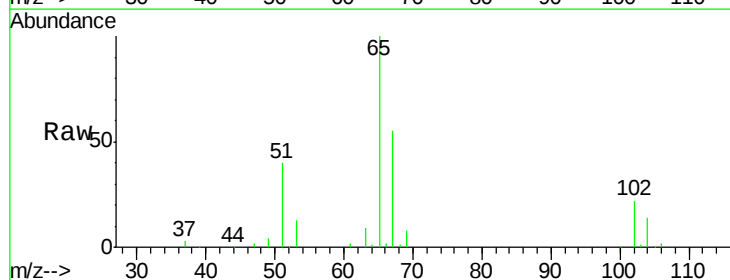

Abundance Ion 64.90 (64.60 to 65.60): VU028994.D (-1270) (-)

Ion 66.90 (66.60 to 67.60): VU028994.D (-1270) (-)




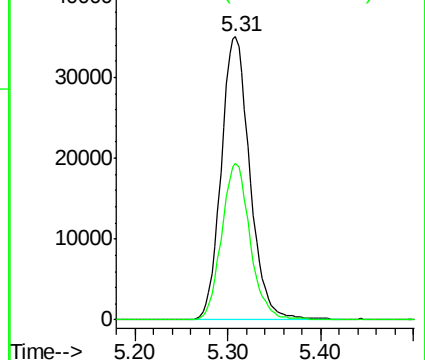




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.88 min Scan# 1465
 Delta R.T. 0.00 min
 Lab File: VU029202.D
 Acq: 16 Jan 2019 12:16




Instrument :
 MSVOA_U
 ClientSampleId :
 TP-4


Tot Ion:114 Resp: 189362
 Ion Ratio Lower Upper
 114 100
 63 20.7 0.0 40.2
 88 15.4 0.0 30.4

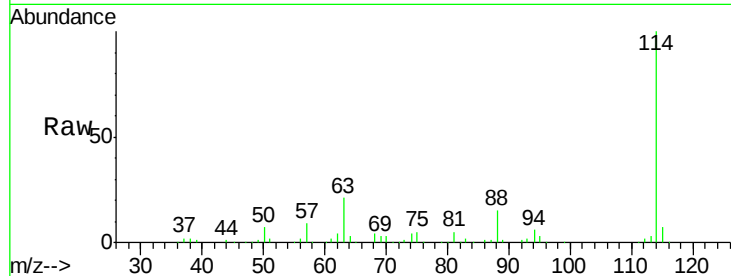

#35
 Dibromofluoromethane
 Concen: 52.572 ug/l
 RT: 4.88 min Scan# 1153
 Delta R.T. 0.00 min
 Lab File: VU029202.D
 Acq: 16 Jan 2019 12:16

Tgt Ion:113 Resp: 64532
 Ion Ratio Lower Upper
 113 100
 111 105.8 81.4 122.2
 192 21.2 16.8 25.2







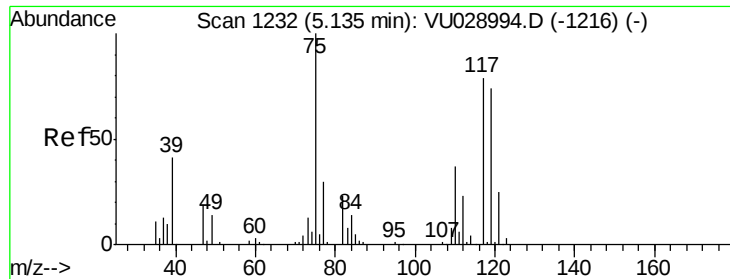

#36
 1,1-Dichloropropene
 Concen: 4.073 ug/l
 RT: 4.98 min Scan# 1183
 Delta R.T. -0.16 min
 Lab File: VU029202.D
 Acq: 16 Jan 2019 12:16




Instrument :
 MSVOA_U
 ClientSampleId :
 TP-4


Tot Ion: 75 Resp: 7710
 Ion Ratio Lower Upper
 75 100
 110 5.8 18.4 55.4#
 77 0.0 25.1 37.7#

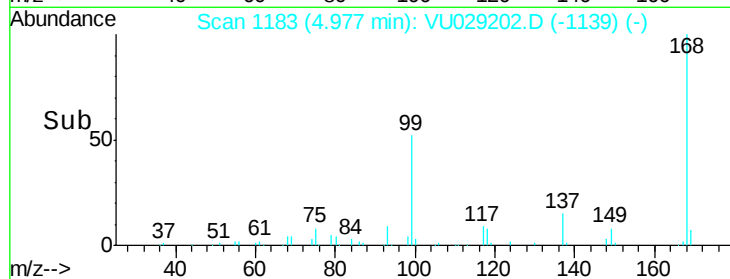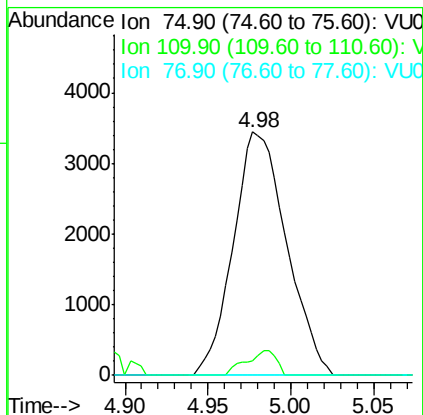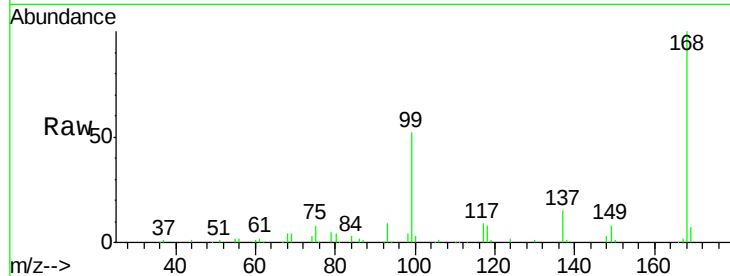

#38
 Carbon Tetrachloride
 Concen: 6.225 ug/l
 RT: 4.98 min Scan# 1184
 Delta R.T. -0.15 min
 Lab File: VU029202.D
 Acq: 16 Jan 2019 12:16

Tgt Ion: 117 Resp: 9827
 Ion Ratio Lower Upper
 117 100
 119 6.1 74.6 111.8#
 121 0.0 25.0 37.6#









#41
Methacrylonitrile
Concen: 0.205 ug/l
RT: 4.66 min Scan# 1085
Delta R.T. 0.12 min
Lab File: VU029202.D
Acq: 16 Jan 2019 12:16




Instrument :
MSVOA_U
ClientSampled :
TP-4


Tot Ion: 41 Resp: 228
Ion Ratio Lower Upper
41 100
39 0.0 42.3 63.5#
67 0.0 64.4 96.6#
52 0.0 23.9 35.9#

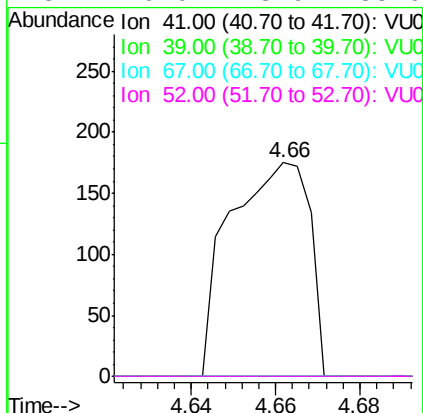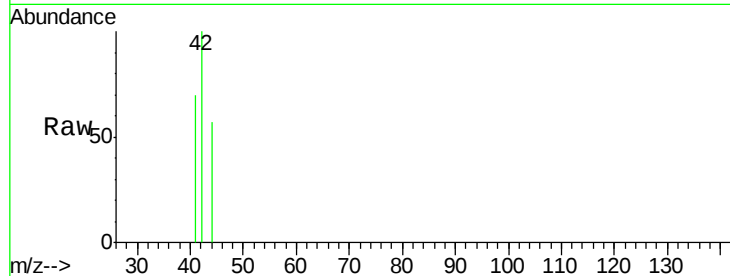

#43
Isopropyl Acetate
Concen: 2.150 ug/l
RT: 5.55 min Scan# 1362
Delta R.T. 0.01 min
Lab File: VU029202.D
Acq: 16 Jan 2019 12:16

Tgt Ion: 43 Resp: 6851
Ion Ratio Lower Upper
43 100
61 19.0 17.8 26.6
87 11.0 11.3 16.9#




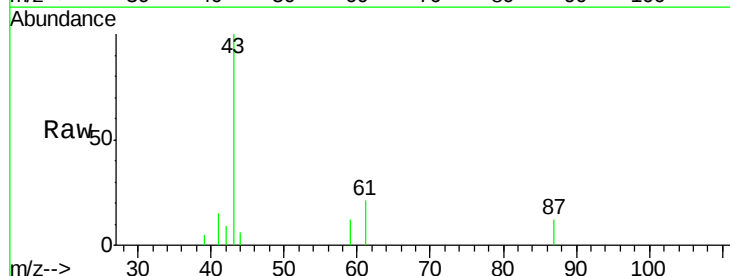


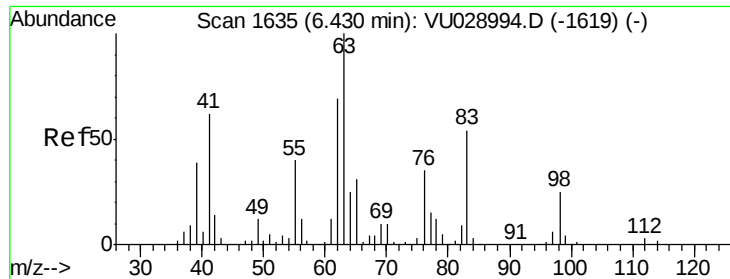

#45
 1,2-Dichloropropane
 Concen: 0.330 ug/l
 RT: 6.70 min Scan# 1719
 Delta R.T. 0.27 min
 Lab File: VU029202.D
 Acq: 16 Jan 2019 12:16




Instrument :
 MSVOA_U
 ClientSampleId :
 TP-4


Tot Ion: 63 Resp: 515
 Ion Ratio Lower Upper
 63 100
 65 0.0 25.1 37.7#

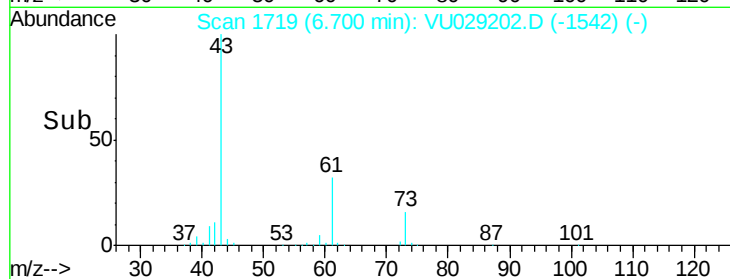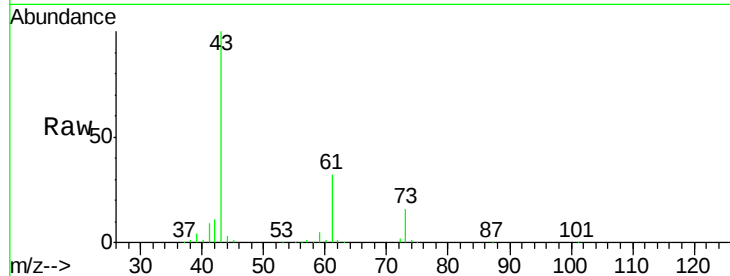

#48
 Methyl methacrylate
 Concen: 25.310 ug/l
 RT: 6.70 min Scan# 1720
 Delta R.T. 0.08 min
 Lab File: VU029202.D
 Acq: 16 Jan 2019 12:16

Tgt Ion: 41 Resp: 39278
 Ion Ratio Lower Upper
 41 100
 69 0.0 73.6 110.4#
 39 48.5 39.6 59.4


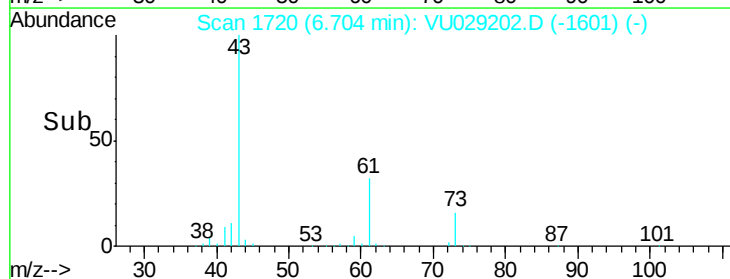






#50
Toluene-d8
Concen: 51.060 ug/l
RT: 7.56 min Scan# 1987
Delta R.T. 0.00 min
Lab File: VU029202.D
Acq: 16 Jan 2019 12:16




Instrument :
MSVOA_U
ClientSampleId :
TP-4


Tot Ion: 98 Resp: 247437
Ion Ratio Lower Upper
98 100
100 64.7 51.6 77.4

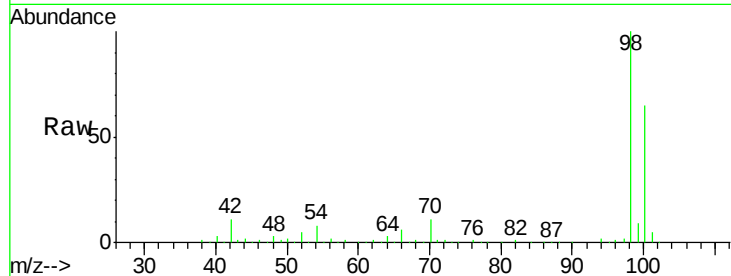

#51
4-Methyl-2-Pentanone
Concen: 16.133 ug/l
RT: 7.42 min Scan# 1942
Delta R.T. -0.04 min
Lab File: VU029202.D
Acq: 16 Jan 2019 12:16

Tgt Ion: 43 Resp: 34992
Ion Ratio Lower Upper
43 100
58 6.9 33.9 50.9#





#52

Toluene

Concen: 0.853 ug/l

RT: 7.64 min Scan# 2011

Delta R.T. 0.00 min

Lab File: VU029202.D

Acq: 16 Jan 2019 12:16

Instrument :

MSVOA_U

ClientSampled :





TP-4

Tot Ion: 92 Resp: 3066

Ion Ratio Lower Upper

92 100

91 195.9 139.8 209.8

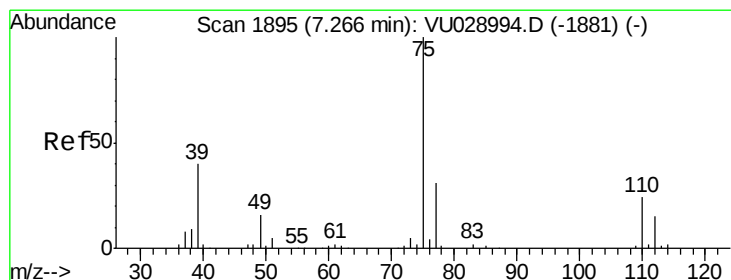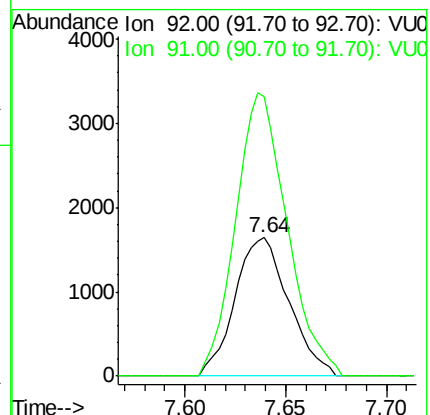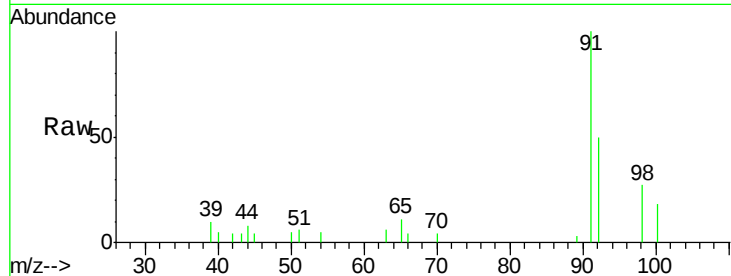

#54

cis-1,3-Dichloropropene

Concen: 7.398 ug/l

RT: 7.42 min Scan# 1942

Delta R.T. 0.15 min

Lab File: VU029202.D

Acq: 16 Jan 2019 12:16




Tgt Ion: 75 Resp: 17623


Ion Ratio Lower Upper

75 100

77 0.0 25.0 37.6#

39 25.7 32.2 48.4#

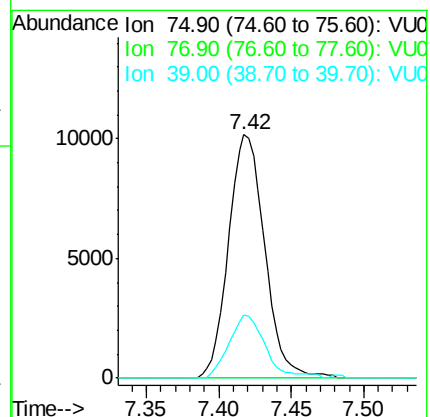



#57

1,3-Dichloropropane

Concen: 1.438 ug/l

RT: 8.41 min Scan# 2252

Delta R.T. 0.17 min

Lab File: VU029202.D

Acq: 16 Jan 2019 12:16

Instrument :

MSVOA_U

ClientSampled :


TP-4

Tot Ion: 76 Resp: 3543

Ion Ratio Lower Upper




76 100

78 0.0 26.0 39.0#

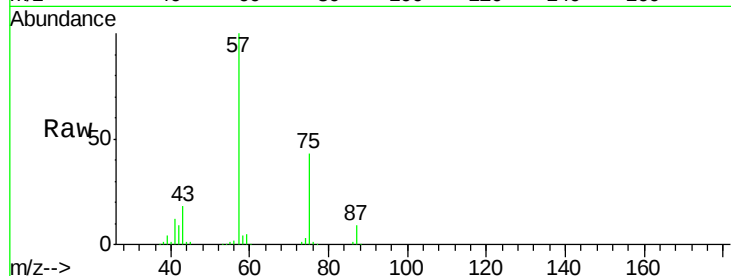

Abundance Ion 75.90 (75.60 to 76.60): VU0

Ion 77.90 (77.60 to 78.60): VU0

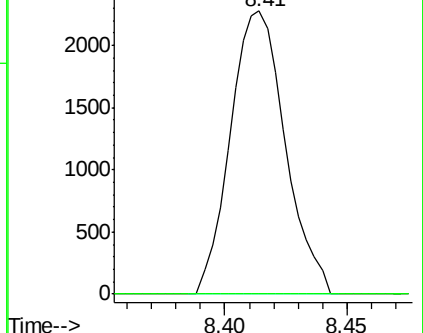

#59

2-Hexanone

Concen: 3.243 ug/l

RT: 8.31 min Scan# 2220

Delta R.T. -0.05 min

Lab File: VU029202.D


Acq: 16 Jan 2019 12:16

Tgt Ion: 43 Resp: 5522

Ion Ratio Lower Upper



43 100


58 0.0 29.8 89.4#



Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

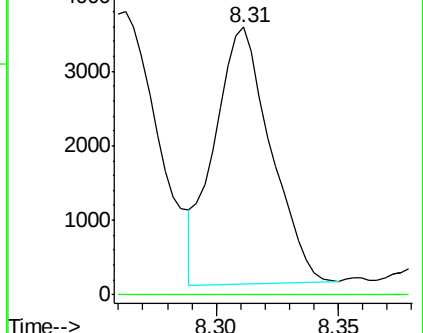



#62

4-Bromofluorobenzene

Concen: 43.599 ug/l

RT: 10.30 min Scan# 2840

Delta R.T. 0.00 min

Lab File: VU029202.D

Acq: 16 Jan 2019 12:16

Instrument :

MSVOA_U

ClientSampleId :

TP-4


Tot Ion: 95 Resp: 75931

Ion Ratio Lower Upper

95 100

174 86.8 0.0 170.6




176 81.4 0.0 165.0



Abundance Ion 94.90 (94.60 to 95.60): VU028994.D (-2828) (-)

Ion 173.80 (173.50 to 174.50): VU028994.D (-2828) (-)

Ion 175.80 (175.50 to 176.50): VU028994.D (-2828) (-)

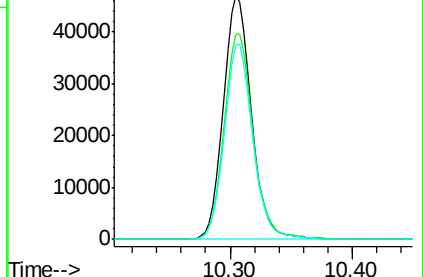

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 9.09 min Scan# 2461

Delta R.T. -0.00 min

Lab File: VU029202.D

Acq: 16 Jan 2019 12:16


Tgt Ion: 117 Resp: 177592

Ion Ratio Lower Upper

117 100

82 56.2 43.9 65.9



119 32.8 26.0 39.0




Abundance Ion 116.90 (116.60 to 117.60): VU028994.D (-2448) (-)

Ion 82.00 (81.70 to 82.70): VU028994.D (-2448) (-)

Ion 118.90 (118.60 to 119.60): VU028994.D (-2448) (-)

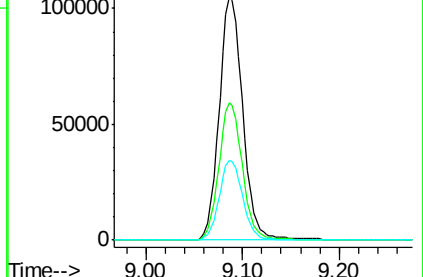

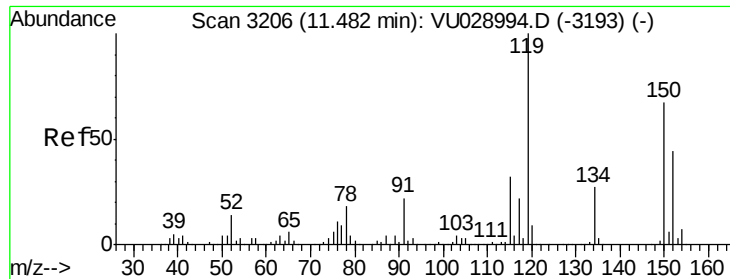

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 11.48 min Scan# 3206

Delta R.T. 0.00 min

Lab File: VU029202.D

Acq: 16 Jan 2019 12:16

Instrument :

MSVOA_U

ClientSampleId :

TP-4


Tot Ion:152 Resp: 70234

Ion Ratio Lower Upper

152 100

115 56.5 40.1 120.3




150 159.2 0.0 345.2

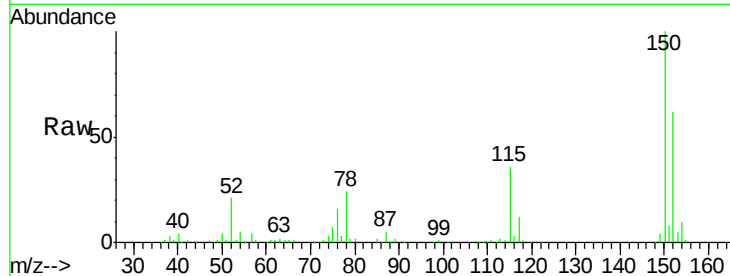

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

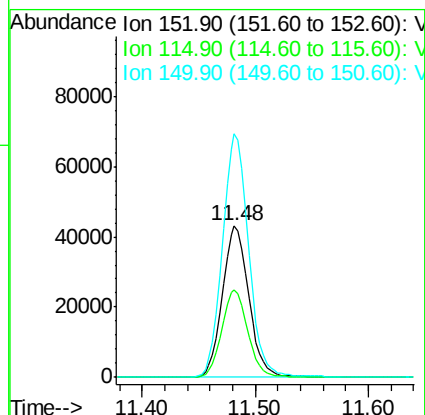

#76

1,2,3-Trichloropropane

Concen: 21.458 ug/l

RT: 10.30 min Scan# 2840

Delta R.T. -0.19 min

Lab File: VU029202.D


Acq: 16 Jan 2019 12:16

Tgt Ion: 75 Resp: 36925

Ion Ratio Lower Upper



75 100


77 1.2 20.9 62.8#



Abundance Ion 74.90 (74.60 to 75.60): VU0

Ion 77.00 (76.70 to 77.70): VU0

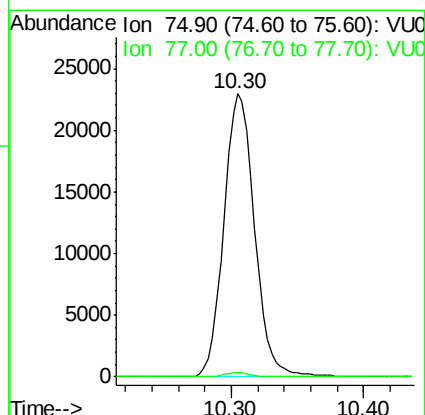



#80

1,3,5-Trimethylbenzene

Concen: 0.311 ug/l

RT: 10.77 min Scan# 2985

Delta R.T. 0.00 min

Lab File: VU029202.D

Acq: 16 Jan 2019 12:16

Instrument :

MSVOA_U

ClientSampled :





TP-4

Tot Ion:105 Resp: 1350

Ion Ratio Lower Upper

105 100

120 41.6 24.8 74.4

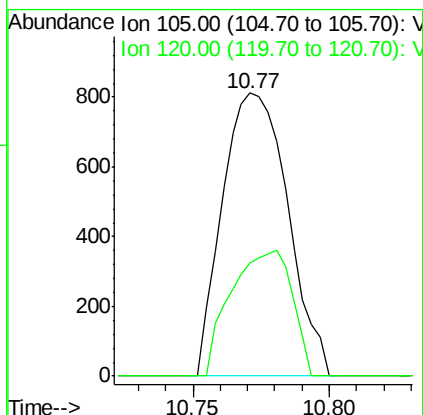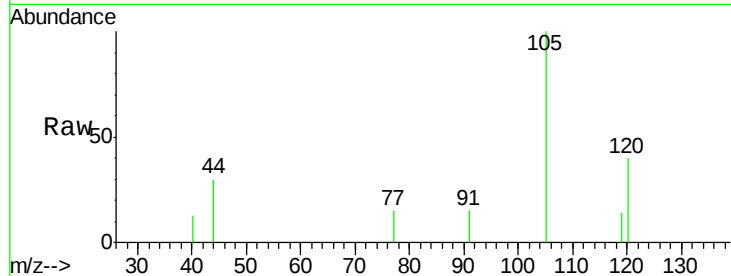

#81

trans-1,4-Dichloro-2-butene

Concen: 55.340 ug/l

RT: 10.30 min Scan# 2840

Delta R.T. -0.21 min

Lab File: VU029202.D

Acq: 16 Jan 2019 12:16

Tgt Ion: 75 Resp: 36925

Ion Ratio Lower Upper

75 100

53 0.0 0.0 0.0

89 0.0 0.0 0.0

