


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU011619\
Data File : VU029194.D
Acq On : 16 Jan 2019 08:39
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U010319W.M
Title : SW846 8260
Last Update : Sat Jan 12 01:33:59 2019

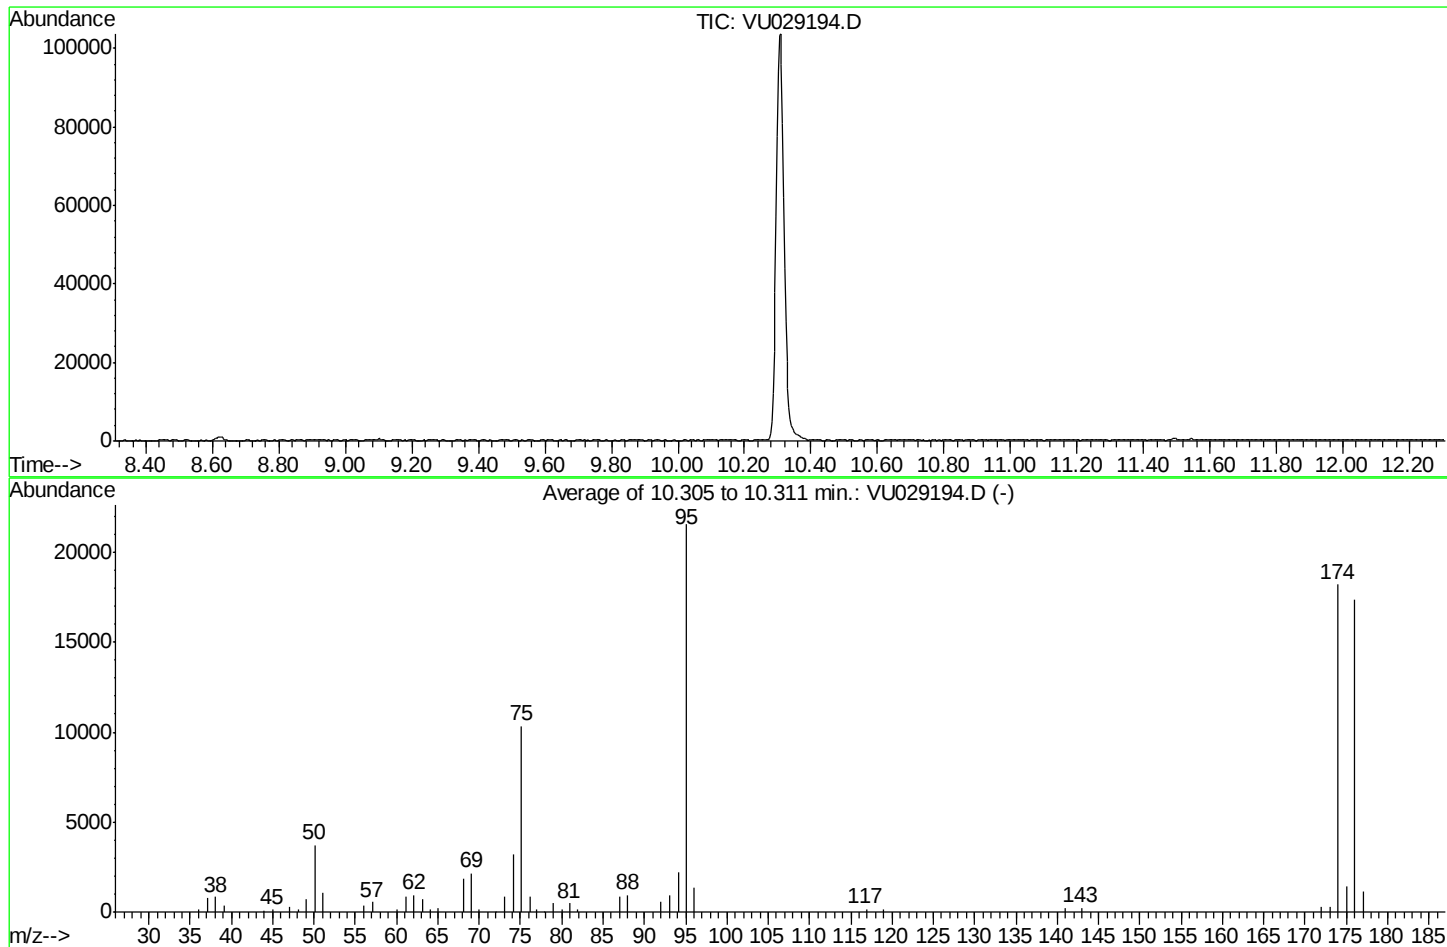

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	3703	PASS
75	95	30	60	47.9	10327	PASS
95	95	100	100	100.0	21557	PASS
96	95	5	9	6.4	1375	PASS
173	174	0.00	2	1.4	258	PASS
174	95	50	100	84.5	18208	PASS
175	174	5	9	7.6	1391	PASS
176	174	95	101	95.2	17338	PASS
177	176	5	9	6.4	1118	PASS