


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU011620\
 Data File : VU036494.D
 Acq On : 16 Jan 2020 10:01
 Operator : JC/MD
 Sample : BFB41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB41

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM011420WMA.M
 Title : VOC Analysis
 Last Update : Fri Jan 17 00:47:08 2020

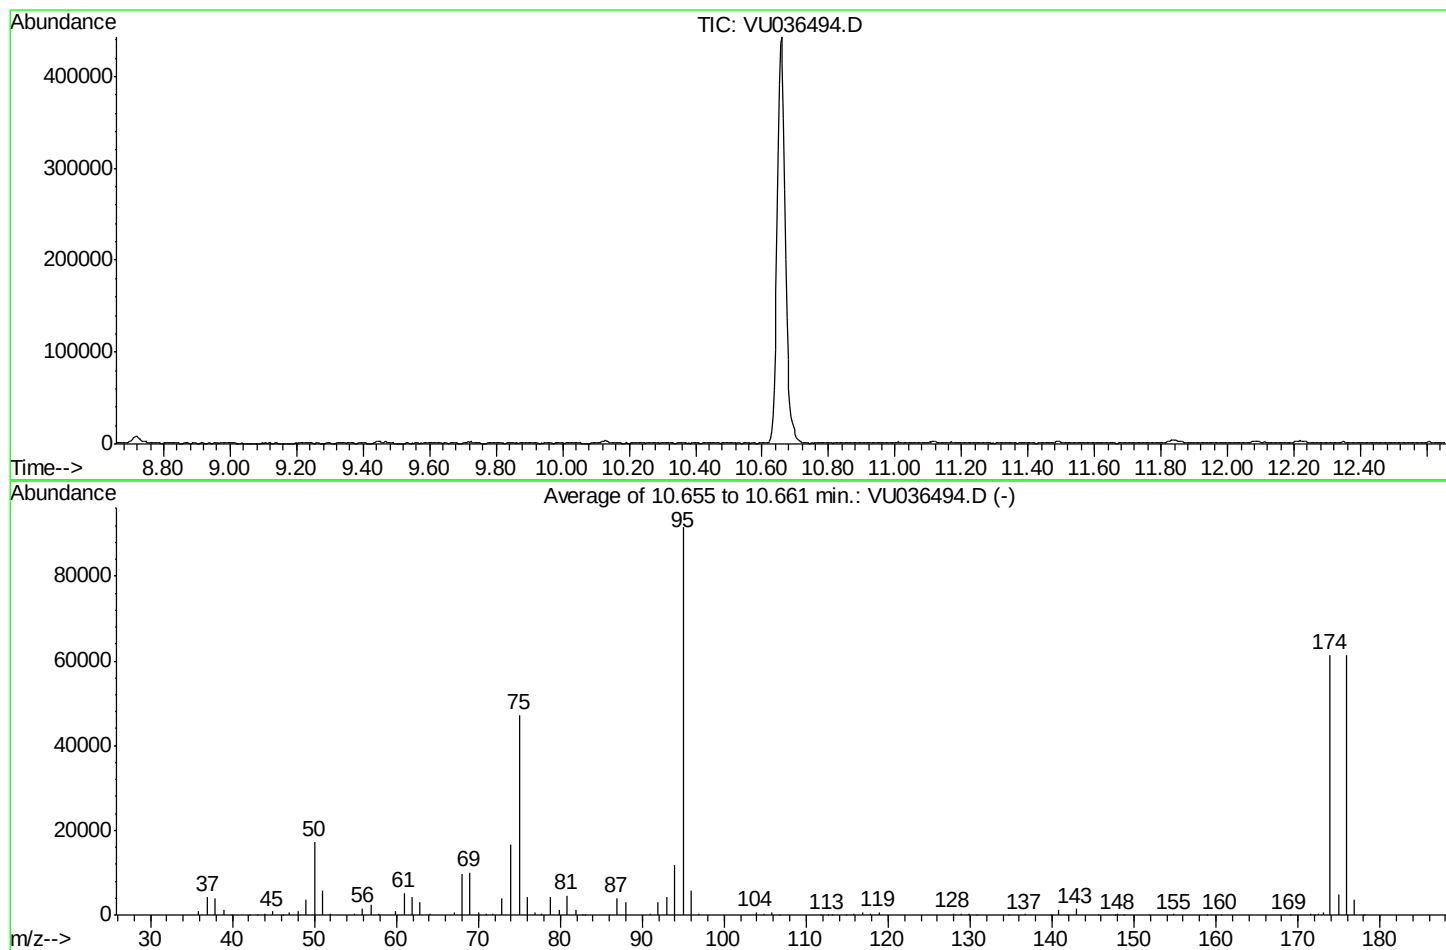

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	17234	PASS
75	95	30	80	51.6	47274	PASS
95	95	100	100	100.0	91546	PASS
96	95	5	9	6.4	5844	PASS
173	174	0.00	2	0.8	507	PASS
174	95	50	120	67.1	61402	PASS
175	174	5	9	7.7	4707	PASS
176	174	95	101	99.8	61296	PASS
177	176	5	9	5.8	3554	PASS

m/z	Abundance
35.90	776.0
36.90	4577.0
37.90	4004.0
38.90	1391.0
40.00	261.0
42.10	112.0
43.00	114.0
44.00	1145.0
44.80	892.0
47.00	752.0
47.90	765.0
49.00	3922.0
50.00	17352.0
51.00	6019.0
51.90	288.0
54.90	251.0
55.90	1533.0
57.00	2794.0
57.90	208.0
59.90	850.0
60.90	5434.0
61.90	4406.0
62.90	3003.0
64.10	336.0
67.00	488.0
67.90	9642.0
68.90	10561.0
70.00	584.0
70.90	112.0
71.80	499.0
72.90	3969.0
73.90	16776.0
75.00	49072.0
76.00	4178.0
76.90	471.0
78.90	4340.0
79.90	1202.0
80.80	4478.0
81.90	1042.0
82.70	127.0
86.90	4103.0
88.00	2939.0
90.90	375.0
92.00	3317.0
92.90	4415.0
94.00	11996.0
95.00	92144.0
96.00	6029.0
96.80	237.0
103.90	619.0
104.90	247.0
105.80	640.0
106.70	127.0
111.80	121.0
114.80	145.0
115.80	358.0
116.90	584.0
117.70	324.0
118.90	497.0
127.90	294.0
128.90	214.0
129.80	358.0
130.90	132.0
134.70	254.0
136.70	251.0
139.80	132.0
140.80	1324.0
142.90	1371.0
148.00	247.0
154.80	226.0
158.90	137.0
160.60	162.0
169.00	146.0
171.40	290.0
172.00	228.0
172.50	439.0
173.00	564.0
173.90	61320.0
174.90	4515.0
175.90	61312.0
176.90	3561.0
177.90	189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
35.80	860.0
36.90	4444.0
37.90	3952.0
39.00	1342.0
40.00	205.0
42.90	164.0
44.00	1098.0
44.80	921.0
46.20	141.0
46.90	768.0
47.90	872.0
49.00	3871.0
50.00	17704.0
50.90	5784.0
51.90	259.0
54.90	339.0
55.90	1579.0
56.90	2606.0
57.90	231.0
59.90	785.0
60.90	5422.0
62.00	4299.0
62.90	3187.0
64.10	430.0
67.00	616.0
68.00	9764.0
68.90	10412.0
70.00	607.0
71.00	204.0
71.80	445.0
72.90	4147.0
74.00	17320.0
75.00	48632.0
76.00	4416.0
76.90	538.0
77.70	345.0
78.80	4435.0
79.90	1332.0
80.80	4712.0
81.90	1159.0
82.80	110.0
86.90	4103.0
87.90	3091.0
90.90	408.0
91.90	2986.0
92.90	4428.0
93.90	12030.0
95.00	94792.0
96.00	5942.0
96.90	230.0
103.90	660.0
104.90	213.0
105.80	574.0
106.80	131.0
111.80	112.0
112.70	109.0
113.10	120.0
114.90	160.0
115.90	386.0
116.90	572.0
117.80	420.0
118.90	662.0
127.90	414.0
128.90	199.0
129.80	391.0
130.80	167.0
134.70	192.0
136.70	252.0
139.80	150.0
140.90	1231.0
142.90	1406.0
148.00	188.0
148.70	104.0
154.90	226.0
158.90	133.0
171.50	311.0
172.60	375.0
173.00	514.0
174.00	62600.0
174.90	4840.0
175.90	63016.0
176.90	3569.0
177.90	126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
35.80	809.0
37.00	4094.0
37.90	3610.0
39.00	1269.0
39.80	211.0
42.90	188.0
43.90	1009.0
44.90	814.0
46.20	127.0
46.90	719.0
48.00	850.0
49.00	3471.0
50.00	16648.0
50.90	5126.0
51.80	223.0
54.90	294.0
55.90	1479.0
56.90	2241.0
57.80	175.0
59.90	758.0
61.00	4943.0
62.00	3977.0
62.90	3341.0
64.10	349.0
67.00	585.0
68.00	9428.0
68.90	9288.0
70.00	667.0
71.00	220.0
71.80	361.0
72.90	3989.0
74.00	15983.0
75.00	44120.0
76.00	4004.0
76.90	605.0
77.70	353.0
78.80	4129.0
79.90	1244.0
80.80	4448.0
81.90	1145.0
83.00	102.0
85.90	143.0
86.90	3636.0
87.90	3346.0
91.00	455.0
92.00	2412.0
93.00	4009.0
94.00	10920.0
95.00	87704.0
96.00	5561.0
96.90	255.0
103.90	642.0
104.90	172.0
105.90	541.0
106.80	162.0
112.60	187.0
113.10	123.0
114.90	172.0
115.90	345.0
116.80	559.0
117.80	450.0
118.90	780.0
128.00	406.0
128.90	173.0
129.90	361.0
130.80	170.0
136.70	198.0
140.90	993.0
141.80	110.0
142.90	1414.0
145.60	117.0
147.70	143.0
148.00	146.0
148.70	152.0
151.90	105.0
155.00	229.0
171.60	311.0
172.60	316.0
173.10	443.0
174.00	60288.0
174.90	4767.0
176.00	59560.0
176.90	3534.0
178.10	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

Scan 2885 (10.616 min): VU036494.D
BFB41

m/z	Abundance
39.80	154.0
43.90	824.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41