

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011623\
 Data File : VU052698.D
 Acq On : 16 Jan 2023 13:07
 Operator : JC/MD
 Sample : 01139-01DL 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH1Y4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052698.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.379	3	12	20	rBV2	8083	14283	2.24%	0.269%
2	1.600	73	81	94	rBV	55158	66924	10.51%	1.261%
3	1.915	170	179	196	rVB	49811	68662	10.79%	1.294%
4	2.571	369	383	399	rBV3	139386	270784	42.54%	5.103%
5	3.044	518	530	549	rBV2	33365	64101	10.07%	1.208%
6	3.867	774	786	802	rVB2	8374	19486	3.06%	0.367%
7	4.648	1011	1029	1064	rBV	73687	289577	45.49%	5.458%
8	5.060	1141	1157	1178	rBV	106793	240922	37.85%	4.541%
9	5.722	1342	1363	1383	rBV2	207116	541112	85.01%	10.198%
10	6.246	1510	1526	1550	rBV	169975	321566	50.52%	6.060%
11	6.539	1602	1617	1637	rBV	339265	636541	100.00%	11.997%
12	6.687	1649	1663	1686	rBV	137157	266010	41.79%	5.013%
13	7.562	1922	1935	1954	rBV	61998	109166	17.15%	2.057%
14	7.896	2025	2039	2057	rBV	236612	412628	64.82%	7.777%
15	8.176	2115	2126	2140	rBV2	37293	63223	9.93%	1.192%
16	8.632	2255	2268	2300	rBV2	309735	612949	96.29%	11.552%
17	9.414	2497	2511	2533	rBV	242924	403083	63.32%	7.597%
18	10.751	2914	2927	2944	rBV	103100	165578	26.01%	3.121%
19	11.809	3244	3256	3282	rBV	234346	372331	58.49%	7.017%
20	12.188	3362	3374	3393	rBV	222473	358961	56.39%	6.765%
21	14.574	4106	4116	4128	rBV2	4550	8083	1.27%	0.152%




Sum of corrected areas: 5305970

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011623\
Data File : VU052698.D
Acq On : 16 Jan 2023 13:07
Operator : JC/MD
Sample : 01139-01DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH1Y4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

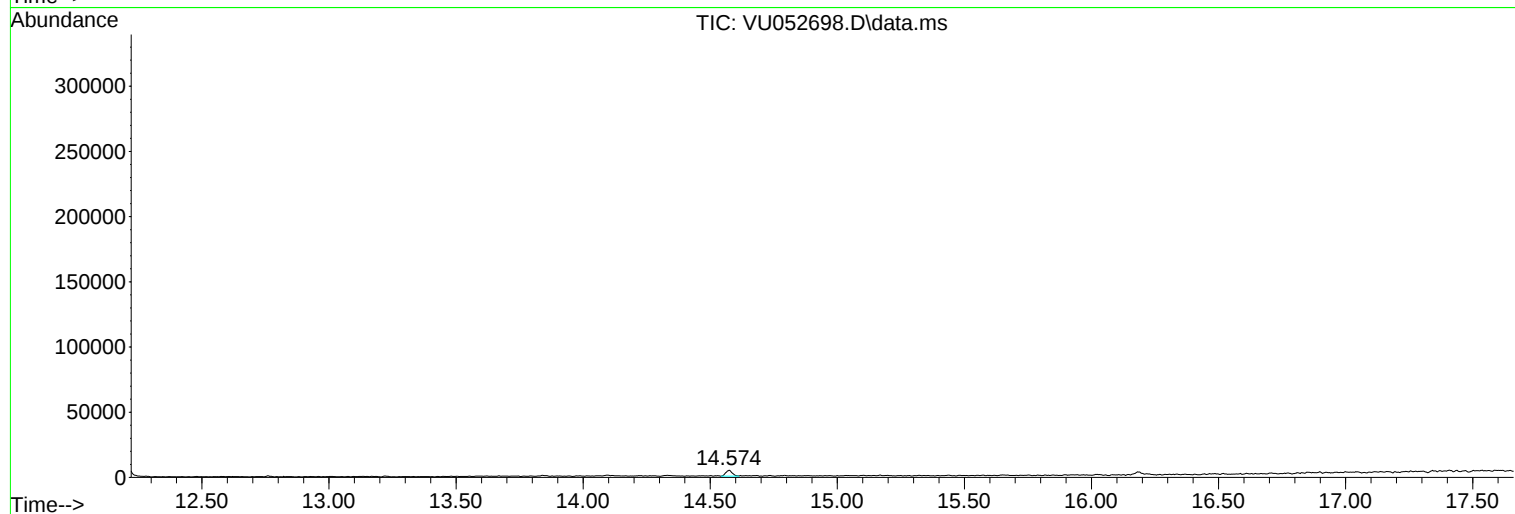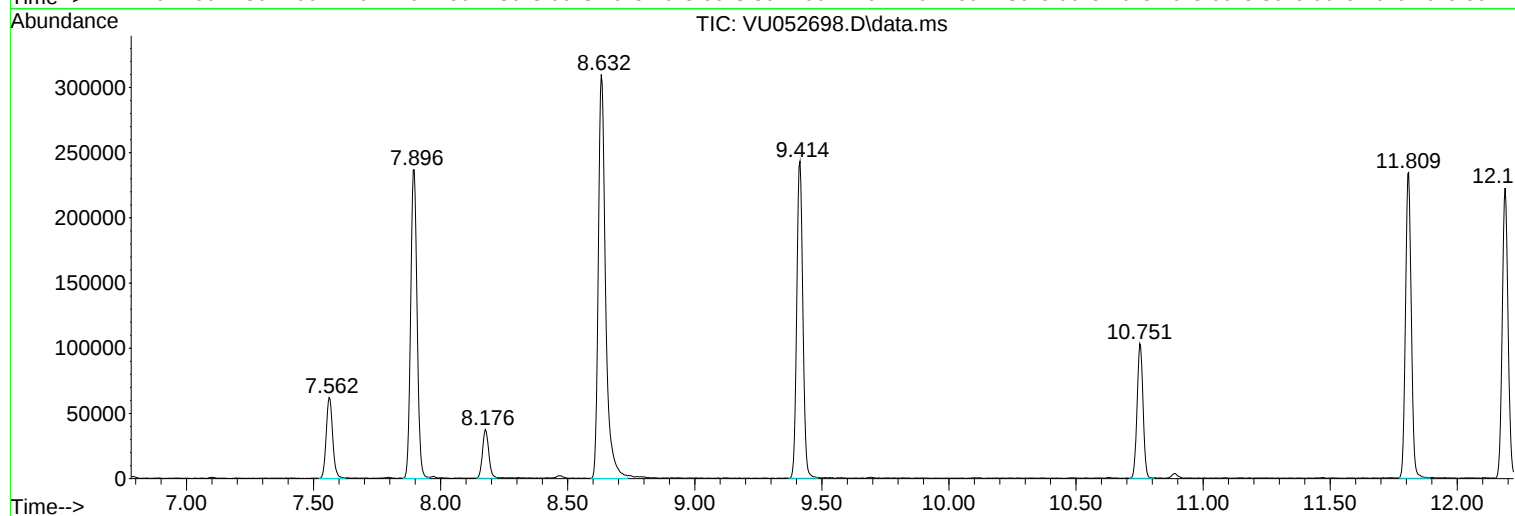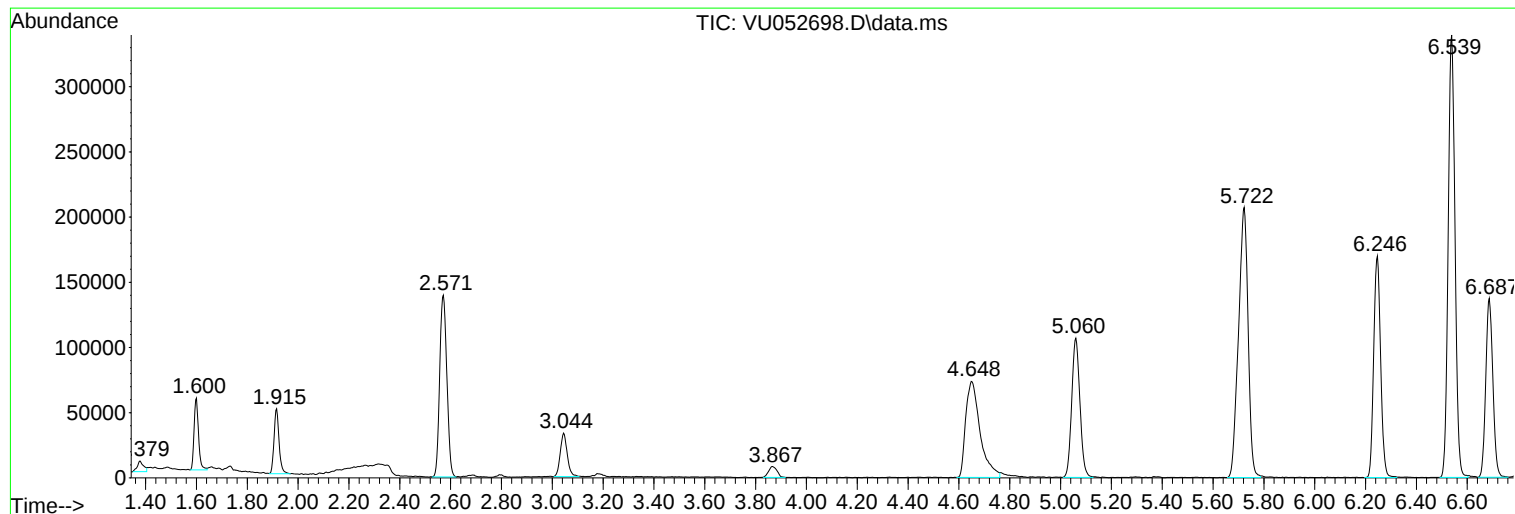

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011623\
Data File : VU052698.D
Acq On : 16 Jan 2023 13:07
Operator : JC/MD
Sample : 01139-01DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH1Y4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011623\
Data File : VU052698.D
Acq On : 16 Jan 2023 13:07
Operator : JC/MD
Sample : 01139-01DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH1Y4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
