

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011623\
 Data File : VU052704.D
 Acq On : 16 Jan 2023 16:33
 Operator : JC/MD
 Sample : 01138-01DL 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH1W4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	71	81	94	rVB	35018	42079	6.99%	1.056%
2	1.732	106	122	126	rBV2	29440	57166	9.50%	1.434%
3	1.916	173	179	191	rVB	30257	39712	6.60%	0.996%
4	2.568	370	382	396	rVB2	77236	135968	22.59%	3.412%
5	2.655	396	409	425	rBV	8719	28535	4.74%	0.716%
6	3.044	516	530	549	rVB3	22730	44269	7.36%	1.111%
7	3.182	563	573	583	rBV3	4696	8892	1.48%	0.223%
8	4.642	1006	1027	1044	rBV3	95784	355475	59.06%	8.920%
9	5.060	1138	1157	1178	rBV2	78866	187743	31.19%	4.711%
10	5.719	1342	1362	1387	rBV2	150173	405452	67.37%	10.174%
11	6.243	1512	1525	1547	rBV	112814	214768	35.68%	5.389%
12	6.539	1601	1617	1634	rBV	161820	301603	50.11%	7.568%
13	6.687	1649	1663	1681	rBV	103455	201574	33.49%	5.058%
14	7.562	1924	1935	1949	rBV2	47231	83632	13.90%	2.099%
15	7.893	2019	2038	2057	rBV	163952	283923	47.17%	7.124%
16	8.176	2113	2126	2142	rBV2	29373	49407	8.21%	1.240%
17	8.632	2248	2268	2300	rBV2	313160	601864	100.00%	15.103%
18	9.414	2498	2511	2536	rVB	167839	276594	45.96%	6.941%
19	10.751	2915	2927	2944	rVB	97782	155694	25.87%	3.907%
20	11.806	3243	3255	3272	rBV	154055	244169	40.57%	6.127%
21	12.188	3362	3374	3392	rBV	165397	266650	44.30%	6.691%




Sum of corrected areas: 3985169

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011623\
Data File : VU052704.D
Acq On : 16 Jan 2023 16:33
Operator : JC/MD
Sample : 01138-01DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH1W4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

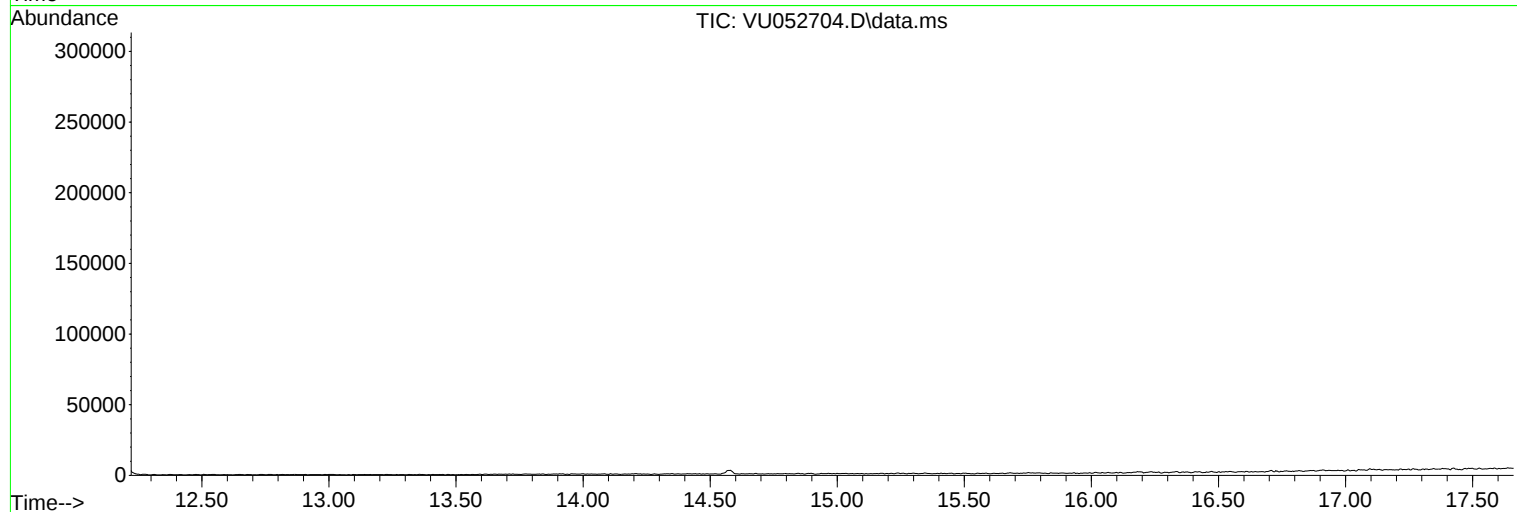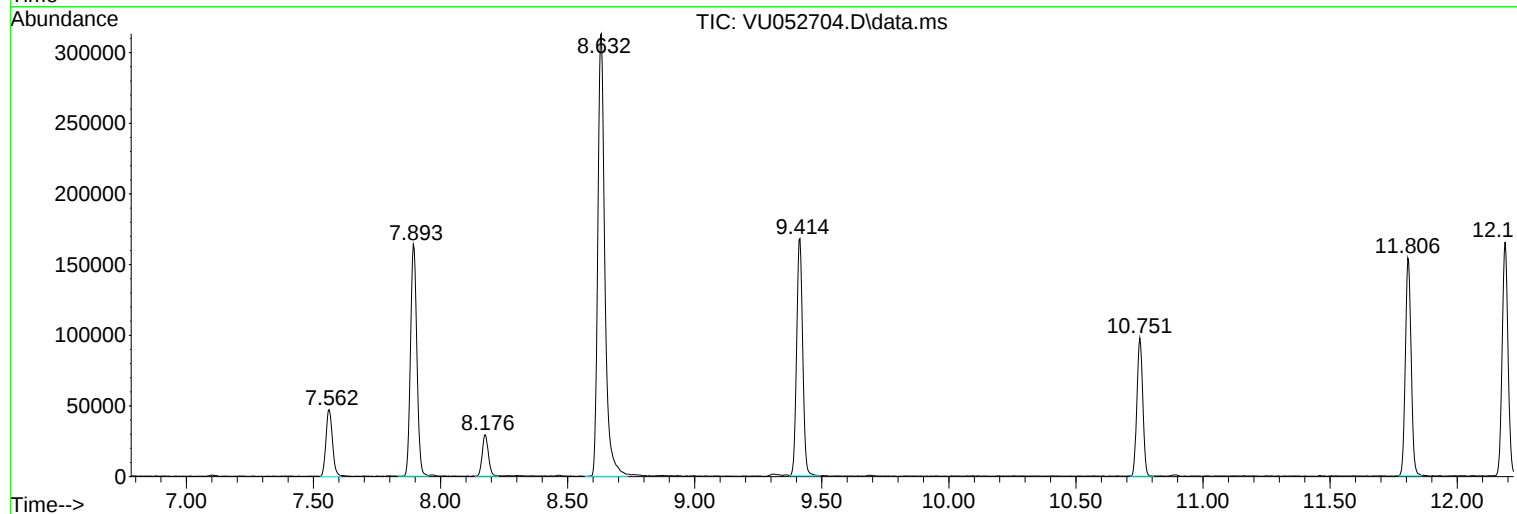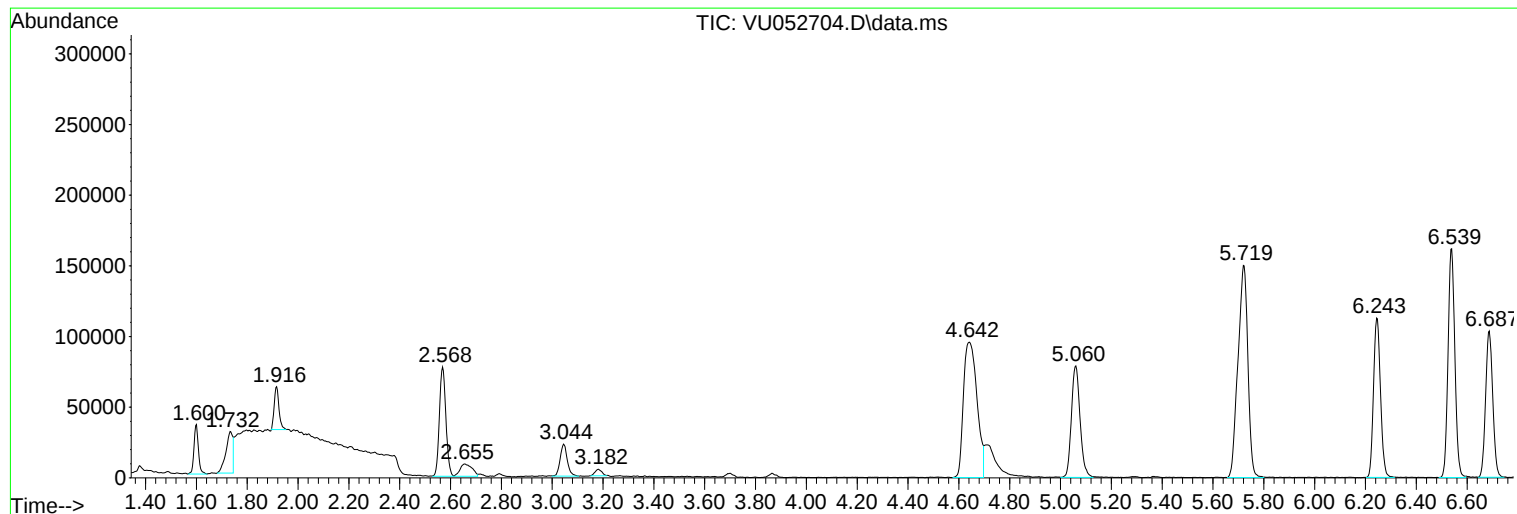

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011623\
Data File : VU052704.D
Acq On : 16 Jan 2023 16:33
Operator : JC/MD
Sample : 01138-01DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH1W4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.732	1.3	ug/L	57166	1	6.243	214768	5.0