
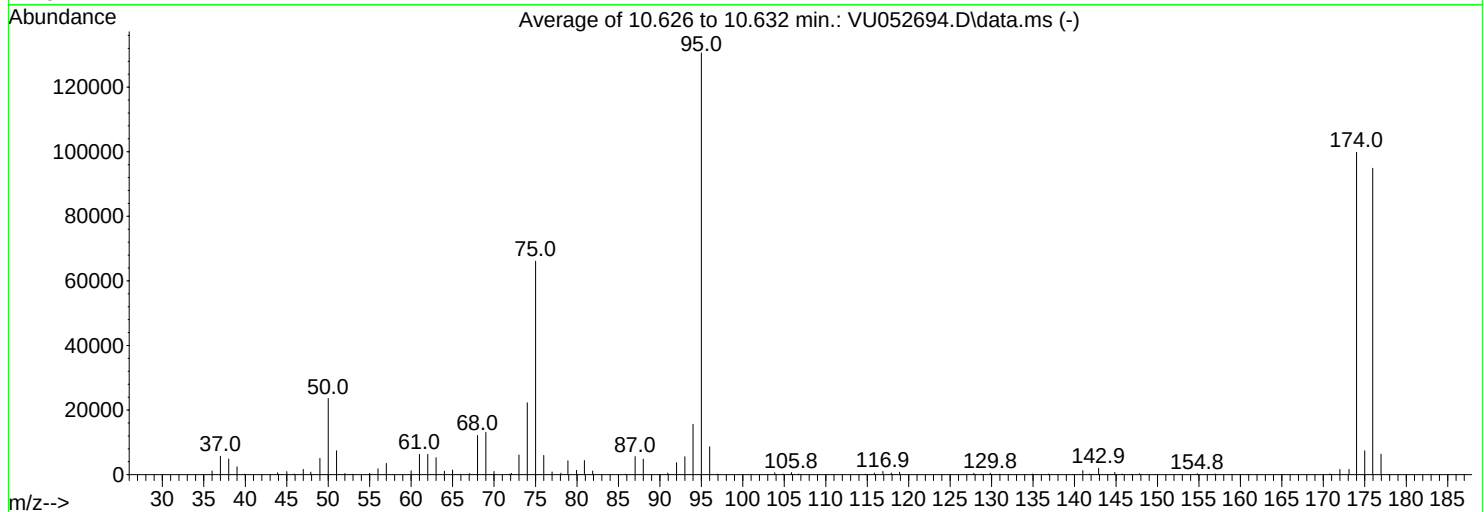


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011623\
 Data File : VU052694.D
 Acq On : 16 Jan 2023 09:39
 Operator : JC/MD
 Sample : BFB190
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB190

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011023WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Jan 18 01:16:13 2023

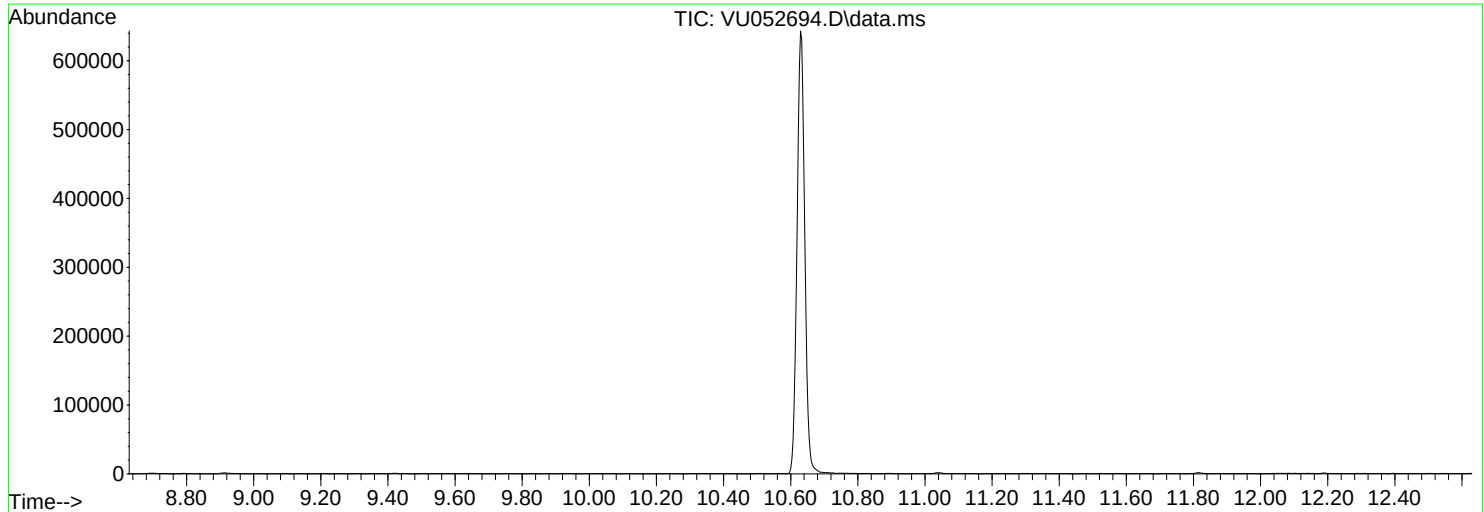

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	23568	PASS
75	95	30	80	50.6	66091	PASS
95	95	100	100	100.0	130621	PASS
96	95	5	9	6.6	8613	PASS
173	174	0.00	2	1.6	1644	PASS
174	95	50	120	76.4	99851	PASS
175	174	5	9	7.4	7361	PASS
176	174	95	101	95.1	94917	PASS
177	176	5	9	6.7	6339	PASS

m/z	Abundance
43.80	248.0

Instrument :
MSVOA_U
ClientSampleId :
BFB190

m/z	Abundance
36.00	1046.0
37.00	5401.0
38.00	4643.0
39.00	2477.0
40.00	215.0
44.00	863.0
45.00	1085.0
45.90	274.0
47.00	1628.0
47.90	723.0
49.00	5111.0
50.00	22704.0
51.00	7250.0
52.00	335.0
52.90	173.0
55.00	385.0
56.00	1717.0
57.00	3481.0
57.80	108.0
60.00	1257.0
61.00	5956.0
62.00	6077.0
63.00	5068.0
64.00	1049.0
65.00	1458.0
66.00	187.0
67.00	379.0
68.00	11378.0
69.00	12267.0
70.00	1003.0
71.90	557.0
73.00	5851.0
74.00	21016.0
75.00	63816.0
76.00	6069.0
77.00	848.0
78.00	495.0
78.90	4274.0
79.90	1337.0
80.90	4283.0
81.90	1083.0
85.80	127.0
87.00	5336.0
88.00	4733.0
90.90	542.0
92.00	3743.0
93.00	5216.0
94.00	14929.0
95.00	123768.0
96.00	8299.0
96.90	137.0
103.90	559.0
104.80	172.0
105.80	585.0
106.70	179.0
114.70	139.0
115.90	498.0
116.90	898.0
117.90	470.0
118.90	767.0
127.80	369.0
128.70	143.0
129.90	441.0
130.90	152.0
134.90	199.0
136.90	194.0
141.00	1131.0
141.90	221.0
142.90	1918.0
144.80	682.0
145.70	193.0
146.90	141.0
147.80	302.0
150.00	143.0
152.90	103.0
154.80	273.0
156.90	230.0
170.80	253.0
172.00	1525.0
173.10	1638.0
174.00	93440.0
175.00	7066.0
176.00	88704.0
177.00	6138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB190

m/z	Abundance
36.00	1185.0
37.00	5982.0
38.00	5025.0
39.00	2537.0
39.90	217.0
43.90	891.0
45.00	921.0
45.90	223.0
47.00	1737.0
47.90	797.0
49.00	5212.0
50.00	24280.0
51.00	7567.0
52.00	346.0
52.90	163.0
55.00	406.0
56.00	1908.0
57.00	3609.0
57.80	102.0
60.00	1215.0
61.00	6565.0
62.00	6589.0
63.00	5484.0
64.00	1174.0
65.00	1478.0
65.90	183.0
67.00	382.0
68.00	12527.0
69.00	13559.0
70.00	1068.0
72.10	569.0
73.00	6335.0
74.00	23104.0
75.00	68168.0
76.00	6255.0
77.00	858.0
78.00	441.0
78.90	4501.0
79.90	1407.0
80.90	4520.0
81.90	1165.0
85.80	144.0
87.00	5903.0
88.00	5001.0
90.90	505.0
92.00	3810.0
93.00	5740.0
94.00	16201.0
95.00	135360.0
96.00	9023.0
96.90	172.0
103.90	604.0
104.80	210.0
105.90	675.0
106.70	191.0
114.70	136.0
115.90	530.0
116.90	1027.0
117.90	508.0
118.90	747.0
127.90	431.0
128.80	162.0
129.90	467.0
131.00	176.0
135.00	220.0
136.90	209.0
141.00	1286.0
141.80	169.0
142.90	2056.0
144.00	104.0
144.80	683.0
145.70	212.0
146.90	136.0
147.80	315.0
150.00	142.0
152.90	126.0
154.80	298.0
156.90	269.0
170.80	274.0
172.00	1682.0
173.10	1712.0
174.00	102904.0
175.00	7559.0
175.90	97712.0
176.90	6538.0
177.90	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB190

m/z	Abundance
36.00	1130.0
37.00	5785.0
38.00	4953.0
39.00	2287.0
39.90	254.0
43.90	839.0
45.00	786.0
45.90	177.0
47.00	1608.0
47.90	833.0
49.00	4820.0
50.00	23720.0
51.00	7377.0
52.00	341.0
52.90	162.0
55.00	367.0
56.00	1884.0
57.00	3332.0
60.00	1084.0
61.00	6414.0
62.00	6243.0
63.00	5263.0
64.00	1046.0
65.00	1379.0
65.90	148.0
67.10	350.0
68.00	12556.0
69.00	13479.0
70.00	951.0
72.10	560.0
73.00	6164.0
74.00	22664.0
75.00	66288.0
76.00	5589.0
77.00	799.0
78.10	452.0
78.90	4151.0
80.00	1333.0
80.90	4296.0
81.90	1129.0
85.90	200.0
87.00	5630.0
88.00	4766.0
91.00	443.0
92.00	3566.0
93.00	5660.0
94.00	15709.0
95.00	132736.0
96.00	8518.0
96.90	221.0
103.80	626.0
104.90	243.0
105.90	697.0
106.80	162.0
114.80	140.0
115.80	536.0
116.90	1032.0
117.90	513.0
118.90	729.0
127.90	479.0
128.90	166.0
129.80	473.0
131.00	172.0
135.00	219.0
136.80	218.0
139.80	104.0
141.00	1289.0
141.70	146.0
142.90	1941.0
144.90	658.0
145.80	254.0
147.90	312.0
152.80	139.0
154.80	291.0
157.00	297.0
160.80	120.0
170.80	280.0
172.00	1571.0
173.10	1581.0
174.00	103208.0
175.00	7459.0
176.00	98336.0
176.90	6342.0
177.90	164.0

Instrument :
MSVOA_U
ClientSampleId :
BFB190