

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011625\
 Data File : VU062809.D
 Acq On : 16 Jan 2025 10:55
 Operator : MD/SY
 Sample : Q1071-17
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GCQ81

Quant Time: Jan 16 22:04:23 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 16 22:02:47 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	97336	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	88903	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	42477	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	15278	2.834	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	56.600%
7) Chloroethane-d5	1.904	69	16562	3.819	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.400%
11) 1,1-Dichloroethene-d2	2.557	65	9267	3.318	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.400%
20) 2-Butanone-d5	4.605	46	62874	57.065	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.140%
24) Chloroform-d	5.049	84	59525	4.488	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.800%
26) 1,2-Dichloroethane-d4	5.689	65	34639	4.815	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.200%
32) Benzene-d6	5.714	84	94495	4.348	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.000%
36) 1,2-Dichloropropane-d6	6.679	67	29276	4.859	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.200%
41) Toluene-d8	7.888	98	86140	4.068	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.400%
43) trans-1,3-Dichloroprop...	8.171	79	14660	4.881	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.600%
46) 2-Hexanone-d5	8.621	63	51905	54.948	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.900%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	27241	5.398	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.000%
66) 1,2-Dichlorobenzene-d4	12.184	152	34949	4.945	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.000%
Target Compounds					Qvalue	
12) 1,1-Dichloroethene	2.570	96	26336	4.359	ug/L	97
17) Methyl tert-butyl Ether	3.351	73	108235	6.518	ug/L	99
19) 1,1-Dichloroethane	3.853	63	76538	6.613	ug/L	92
22) cis-1,2-Dichloroethene	4.653	96	42902	6.086	ug/L	95
34) Trichloroethene	6.534	95	3318	0.380	ug/L	92
70) 1,2,4-trichlorobenzene	13.839	180	6835	0.830	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011625\
Data File : VU062809.D
Acq On : 16 Jan 2025 10:55
Operator : MD/SY
Sample : Q1071-17
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GCQ81

Quant Time: Jan 16 22:04:23 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 16 22:02:47 2025
Response via : Initial Calibration




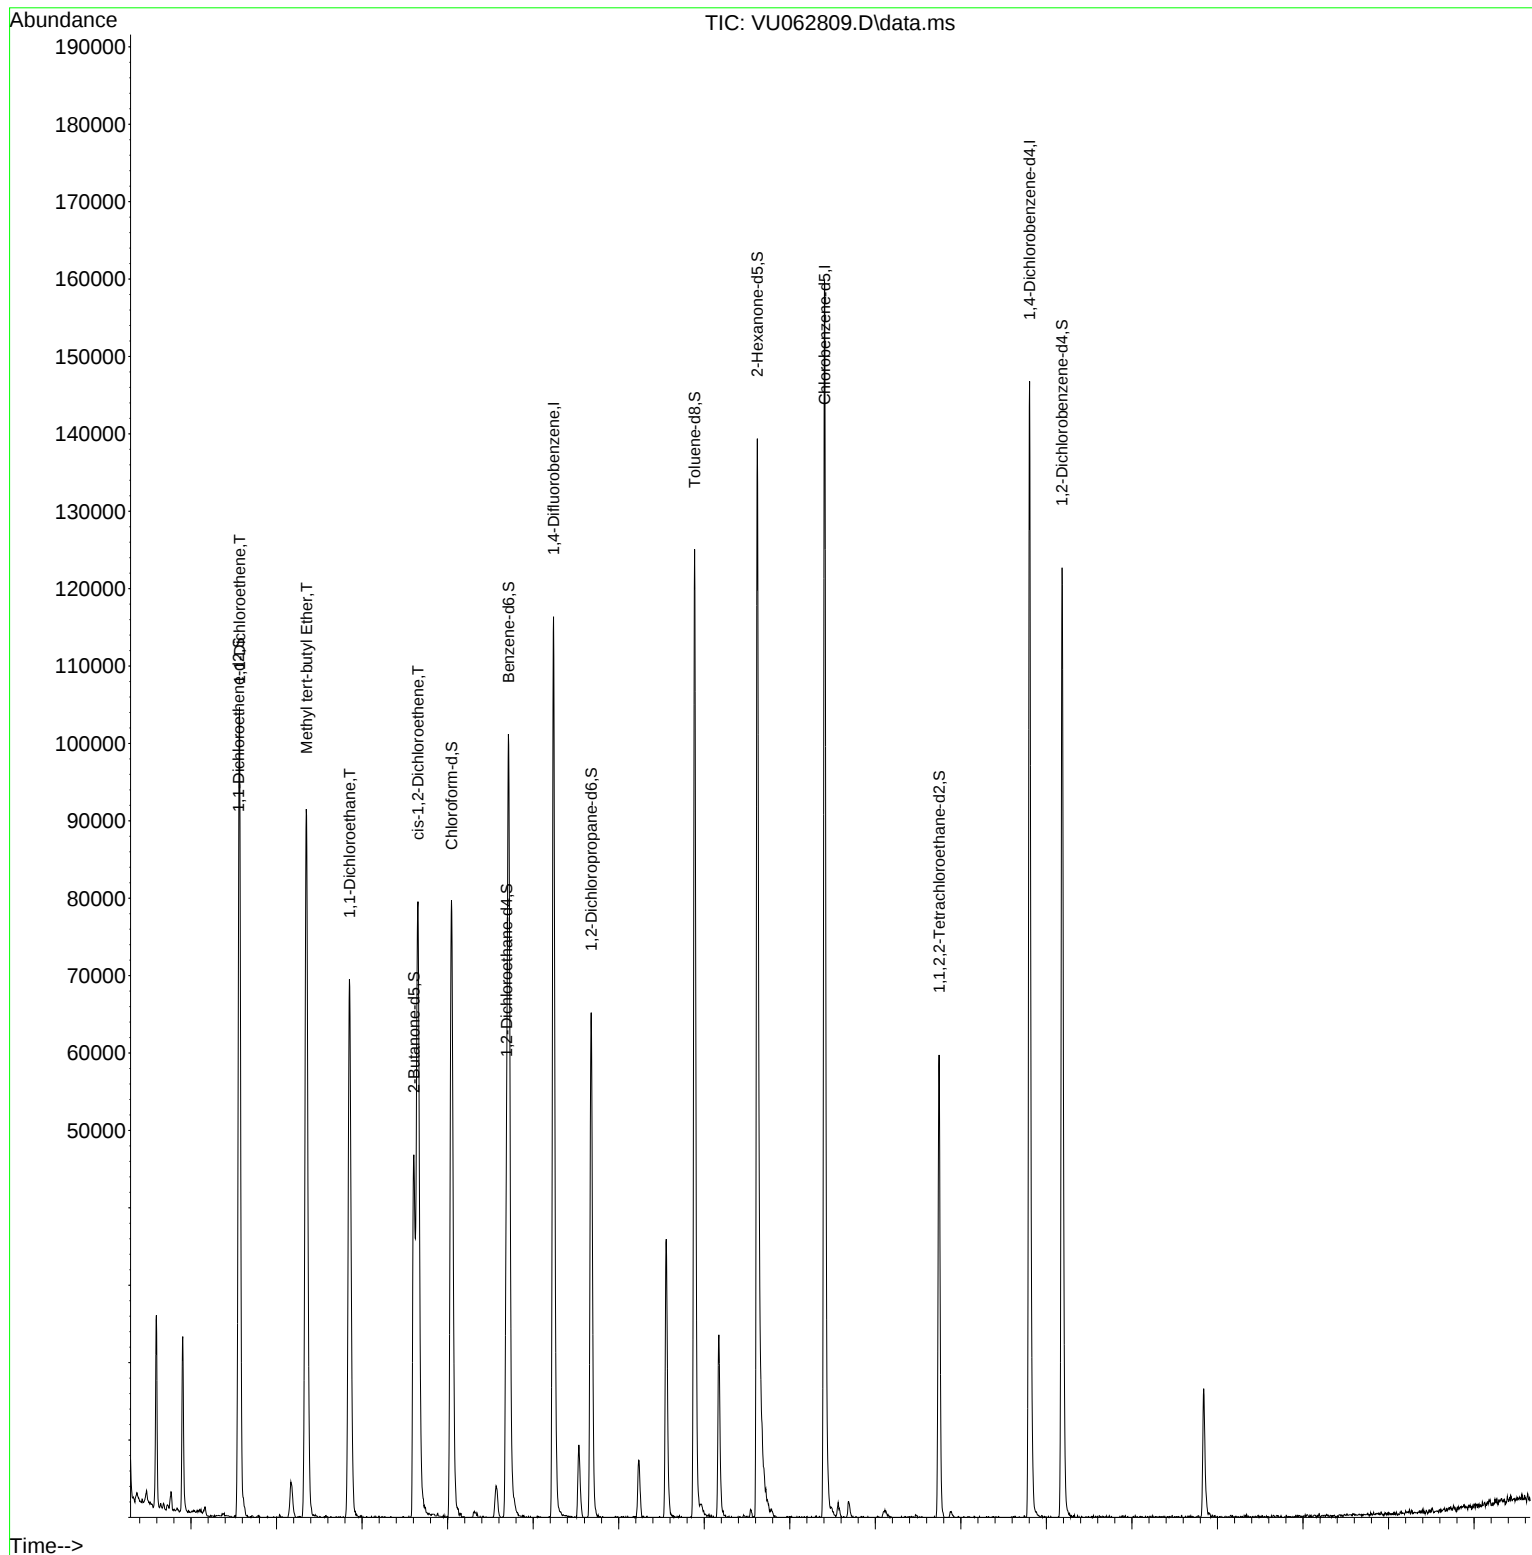


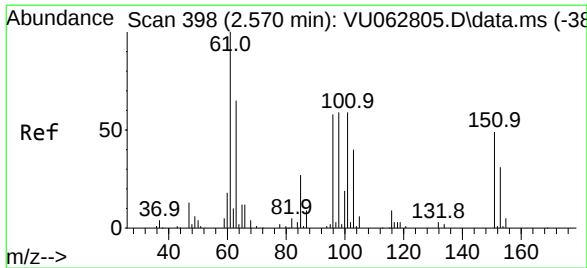

#12
1,1-Dichloroethene
Concen: 4.359 ug/L
RT: 2.570 min Scan# 39
Delta R.T. 0.000 min
Lab File: VU062809.D
Acq: 16 Jan 2025 10:55




Instrument :
MSVOA_U
ClientSampleId :
GCQ81


Tgt Ion: 96 Resp: 26336
Ion Ratio Lower Upper
96 100
61 167.6 120.4 223.6
63 113.8 82.3 152.9

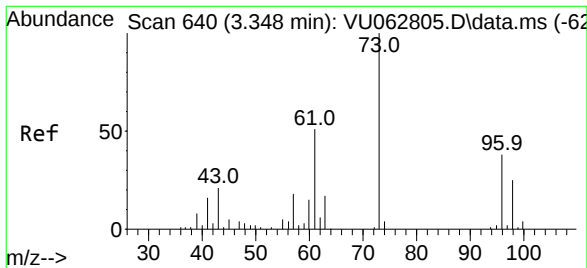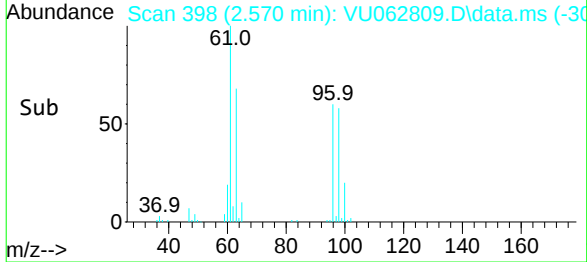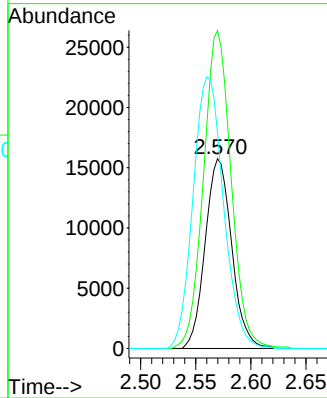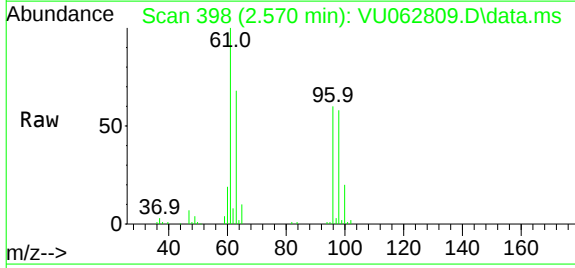

#17
Methyl tert-butyl Ether
Concen: 6.518 ug/L
RT: 3.351 min Scan# 641
Delta R.T. 0.003 min
Lab File: VU062809.D
Acq: 16 Jan 2025 10:55

Tgt Ion: 73 Resp: 108235
Ion Ratio Lower Upper
73 100
43 20.7 16.2 24.4
57 18.6 14.6 22.0


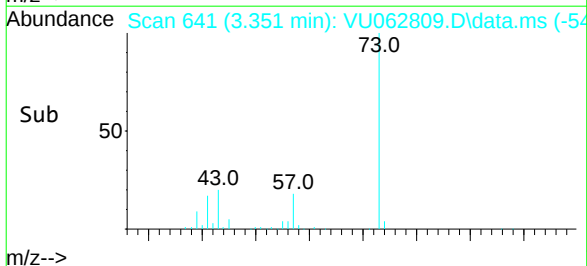
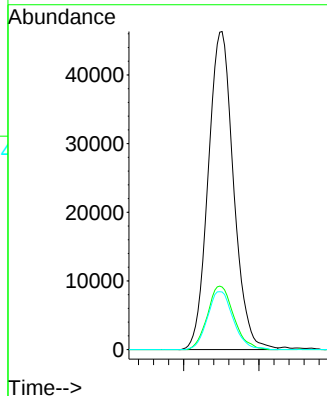
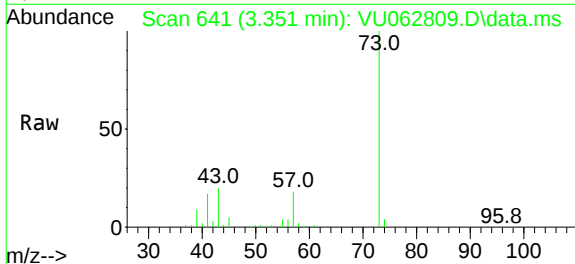


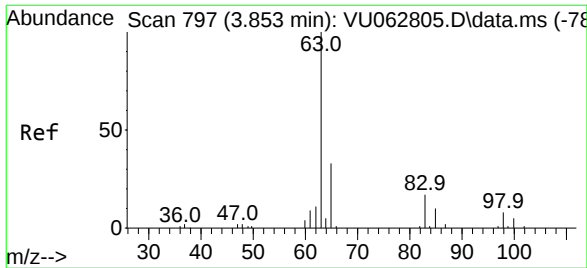

#19
1,1-Dichloroethane
Concen: 6.613 ug/L
RT: 3.853 min Scan# 797
Delta R.T. 0.000 min
Lab File: VU062809.D
Acq: 16 Jan 2025 10:55




Instrument :
MSVOA_U
ClientSampleId :
GCQ81


Tgt Ion:	63	Resp:	76538
Ion	Ratio	Lower	Upper
63	100		
65	34.3	20.7	38.5
83	17.4	10.5	19.5

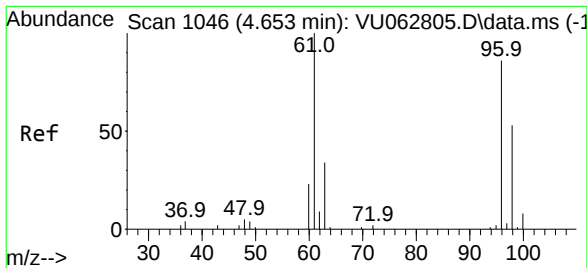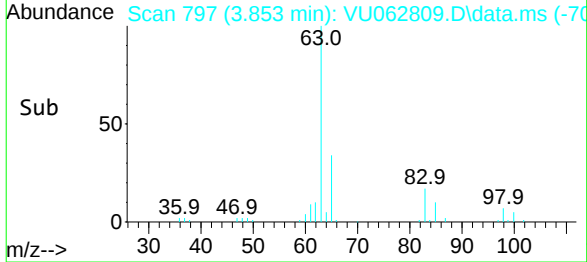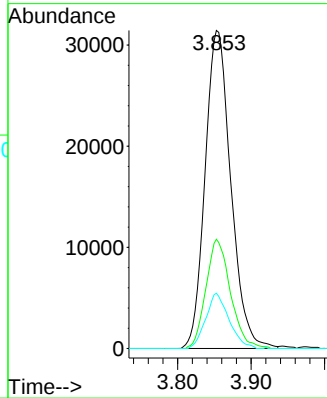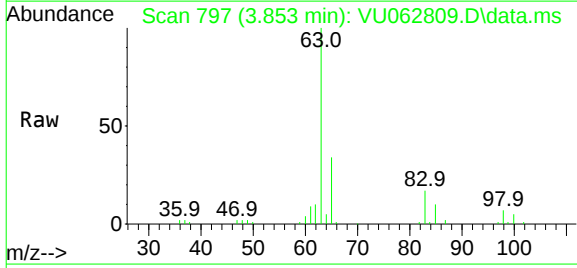

#22
cis-1,2-Dichloroethene
Concen: 6.086 ug/L
RT: 4.653 min Scan# 1046
Delta R.T. 0.000 min
Lab File: VU062809.D
Acq: 16 Jan 2025 10:55

Tgt Ion:	96	Resp:	42902
Ion	Ratio	Lower	Upper
96	100		
61	123.5	84.8	157.6
98	69.2	43.1	80.1


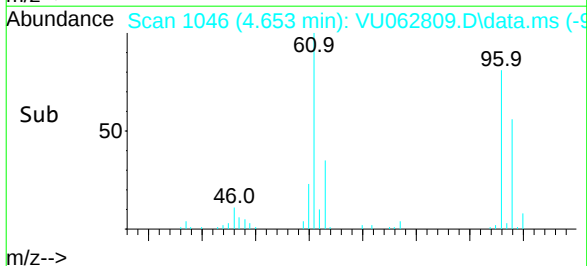
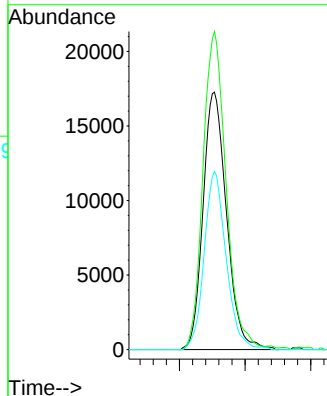
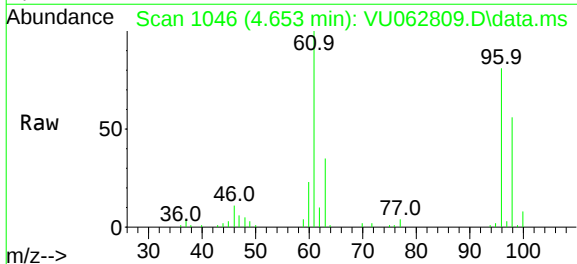


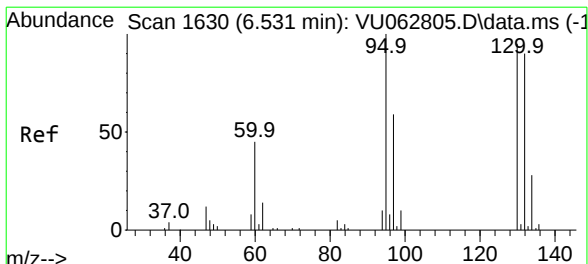

#34
 Trichloroethene
 Concen: 0.380 ug/L
 RT: 6.534 min Scan# 16
 Delta R.T. 0.003 min
 Lab File: VU062809.D
 Acq: 16 Jan 2025 10:55

Instrument :
 MSVOA_U
 ClientSampleId :
 GCQ81

Tgt Ion:	95	Resp:	3318
Ion	Ratio	Lower	Upper
95	100		
97	57.8	47.5	88.3
132	101.7	66.9	124.3
130	91.7	68.6	127.4

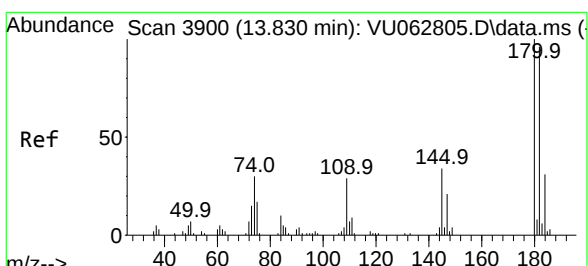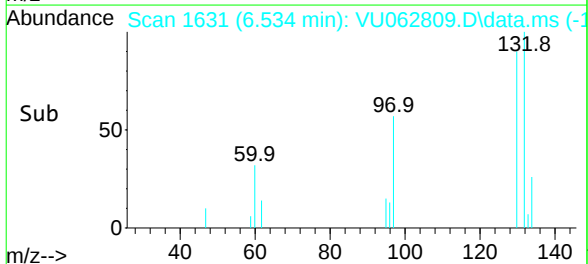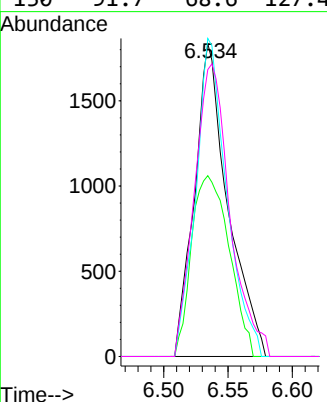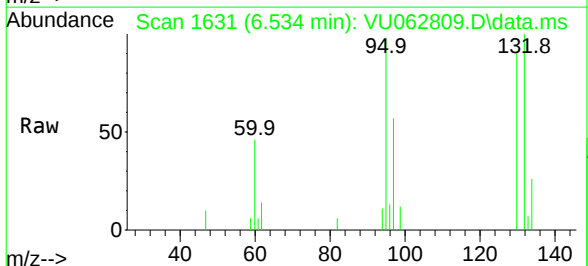

#70
 1,2,4-trichlorobenzene
 Concen: 0.830 ug/L
 RT: 13.839 min Scan# 3903
 Delta R.T. 0.010 min
 Lab File: VU062809.D
 Acq: 16 Jan 2025 10:55

Tgt Ion:	180	Resp:	6835
Ion	Ratio	Lower	Upper
180	100		
182	100.9	77.1	115.7
145	32.8	26.9	40.3

