

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011625\
 Data File : VU062835.D
 Acq On : 16 Jan 2025 21:50
 Operator : MD/SY
 Sample : Q1057-20DL 4X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH8W9DL

Quant Time: Jan 17 00:07:06 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jan 16 23:11:57 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	111337	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	102515	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	50003	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	11975	1.942	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	38.800%#
7) Chloroethane-d5	1.901	69	12541	2.528	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	50.600%#
11) 1,1-Dichloroethene-d2	2.557	65	7181	2.248	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	45.000%#
20) 2-Butanone-d5	4.602	46	57629	45.727	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.460%
24) Chloroform-d	5.049	84	50481	3.327	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	66.600%#
26) 1,2-Dichloroethane-d4	5.689	65	29619	3.599	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.000%
32) Benzene-d6	5.714	84	74505	2.973	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	59.400%#
36) 1,2-Dichloropropane-d6	6.676	67	23064	3.320	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	66.400%
41) Toluene-d8	7.888	98	68381	2.801	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	56.000%#
43) trans-1,3-Dichloroprop...	8.171	79	10867	3.138	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	62.800%
46) 2-Hexanone-d5	8.621	63	43965	40.362	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.720%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	23083	3.967	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	79.400%
66) 1,2-Dichlorobenzene-d4	12.187	152	30089	3.617	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	72.400%#
Target Compounds					Qvalue	
12) 1,1-Dichloroethene	2.570	96	10896	1.576	ug/L	90
19) 1,1-Dichloroethane	3.856	63	4389	0.332	ug/L #	82
21) 2-Butanone	4.692	43	10585	7.961	ug/L	96
22) cis-1,2-Dichloroethene	4.650	96	40704	5.048	ug/L	98
34) Trichloroethene	6.531	95	11943	1.187	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU011625\
Data File : VU062835.D
Acq On : 16 Jan 2025 21:50
Operator : MD/SY
Sample : Q1057-20DL 4X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH8W9DL

Quant Time: Jan 17 00:07:06 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jan 16 23:11:57 2025
Response via : Initial Calibration




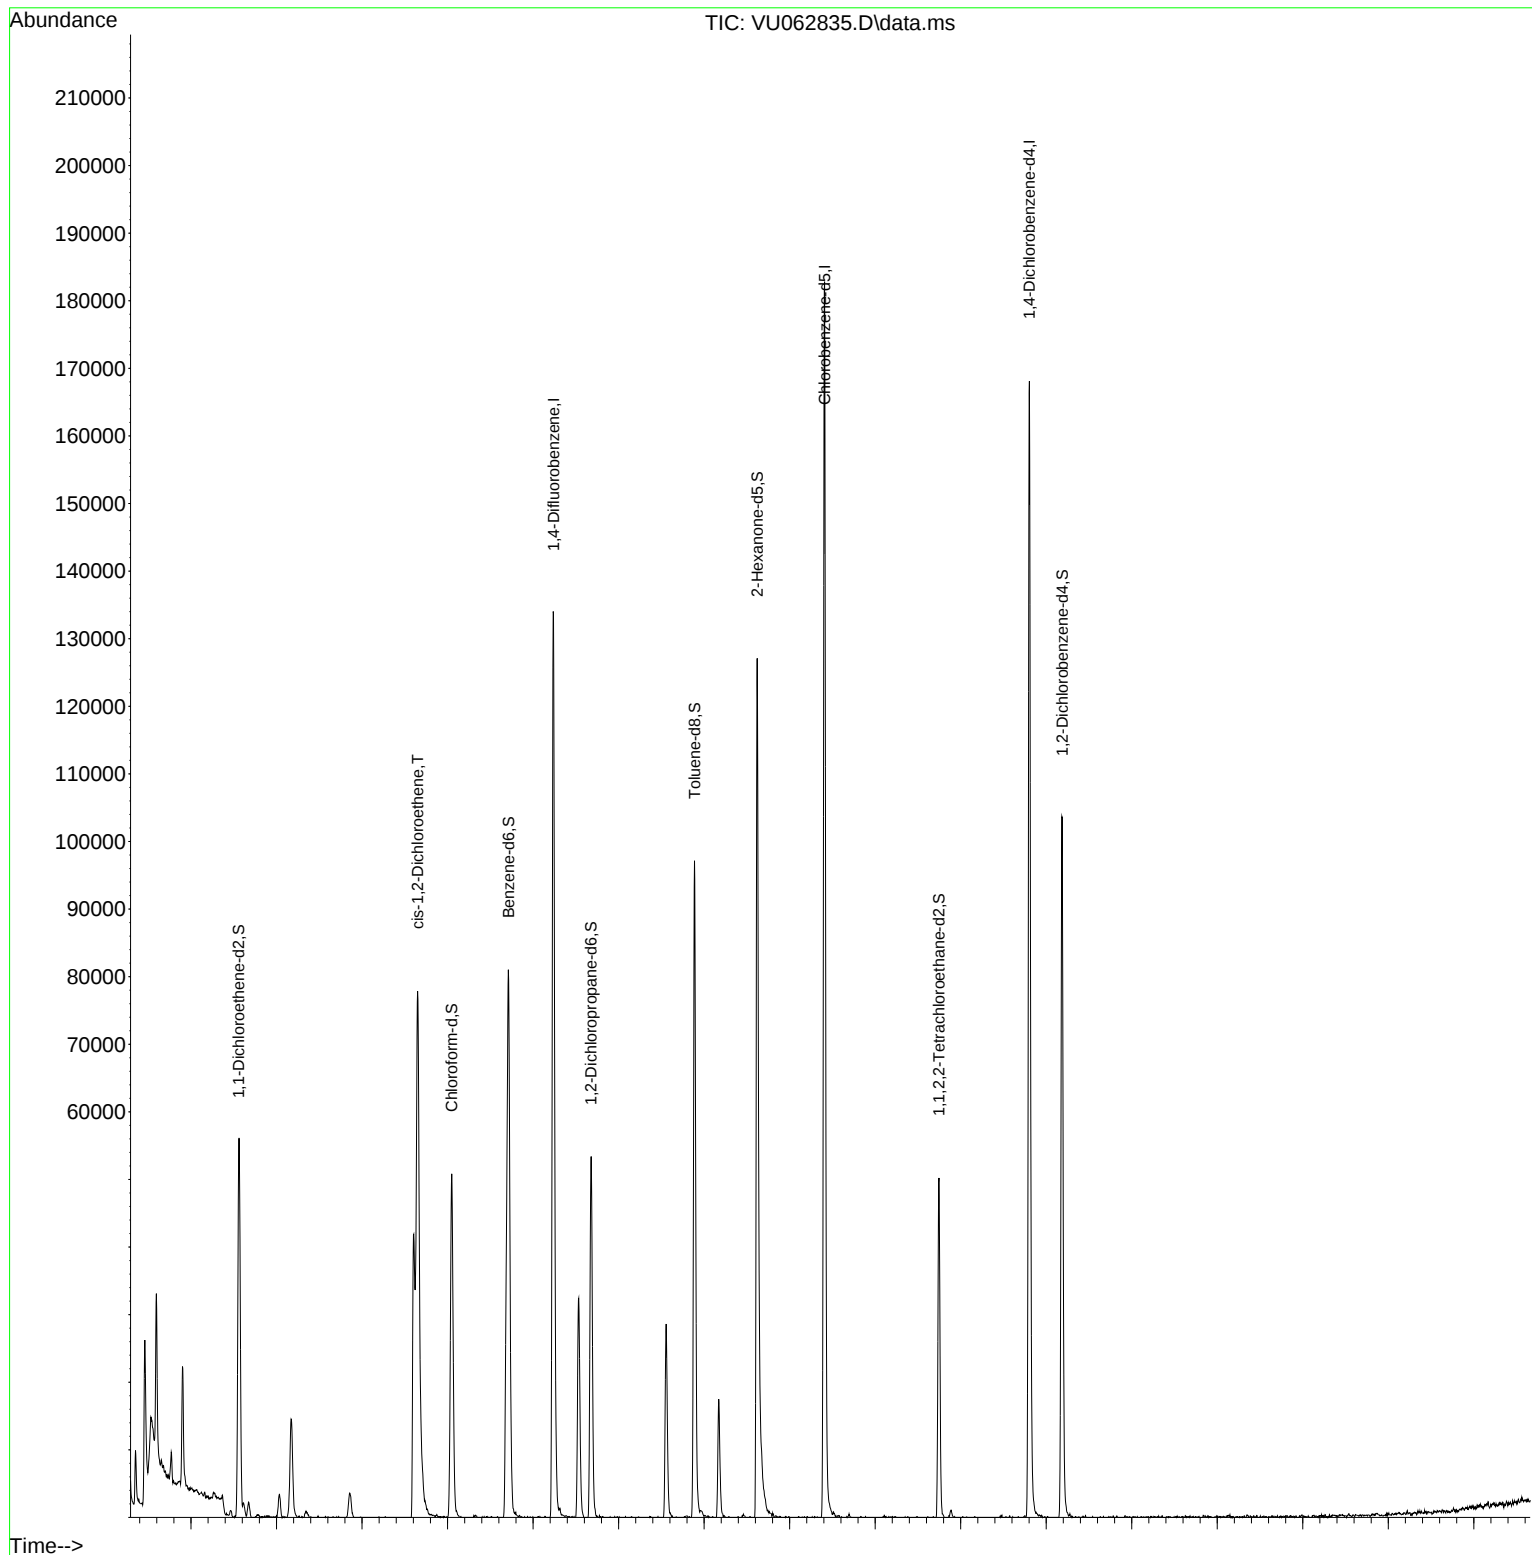


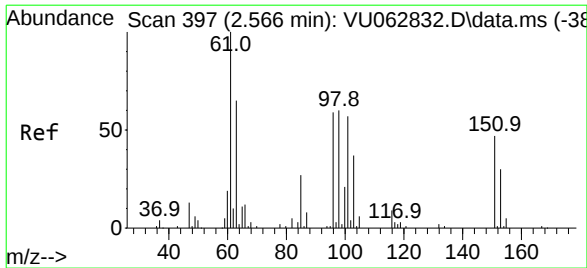

#12
1,1-Dichloroethene
Concen: 1.576 ug/L
RT: 2.570 min Scan# 397
Delta R.T. 0.003 min
Lab File: VU062835.D
Acq: 16 Jan 2025 21:50




Instrument :
MSVOA_U
ClientSampleId :
BH8W9DL


Tgt Ion: 96 Resp: 10896
Ion Ratio Lower Upper
96 100
61 170.0 120.4 223.6
63 141.9 82.3 152.9

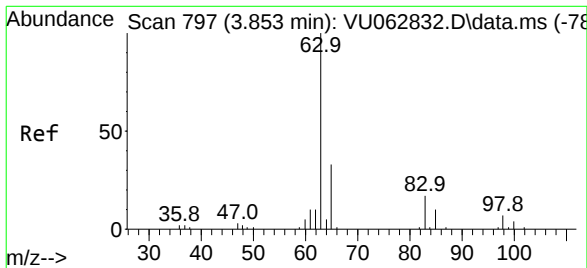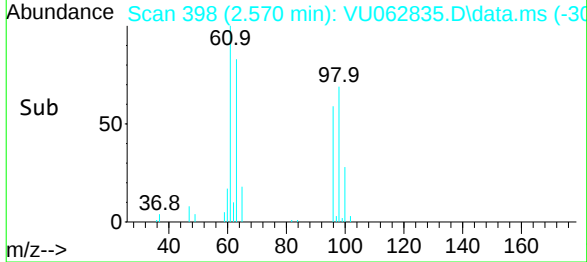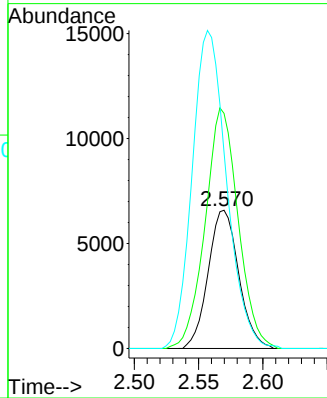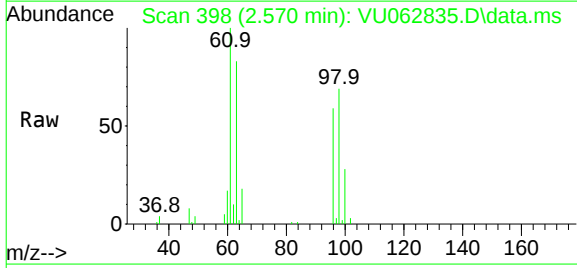

#19
1,1-Dichloroethane
Concen: 0.332 ug/L
RT: 3.856 min Scan# 798
Delta R.T. 0.003 min
Lab File: VU062835.D
Acq: 16 Jan 2025 21:50

Tgt Ion: 63 Resp: 4389
Ion Ratio Lower Upper
63 100
65 44.0 20.7 38.5#
83 15.4 10.5 19.5


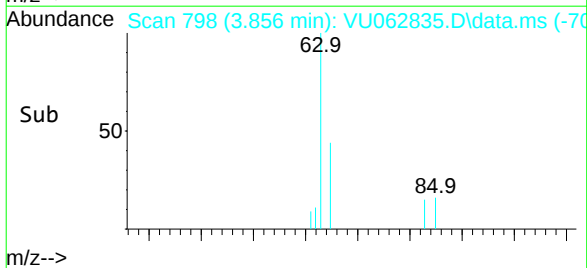
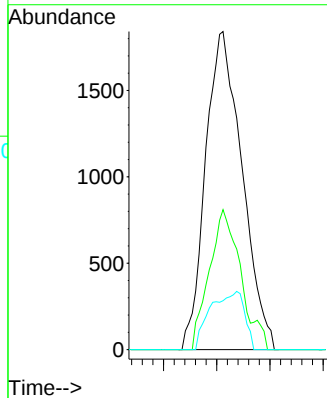
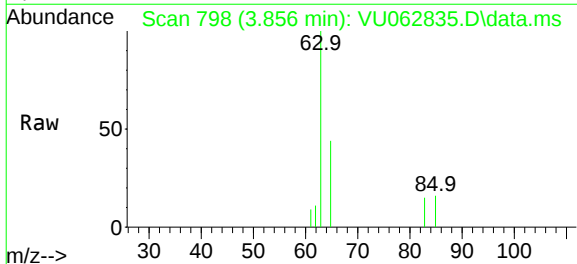


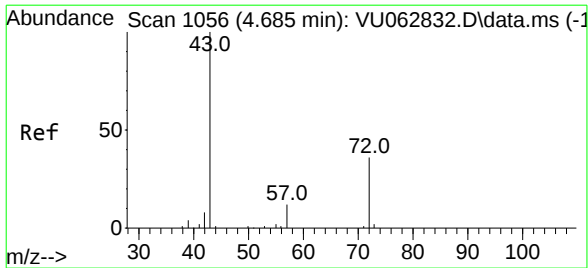

#21
2-Butanone
Concen: 7.961 ug/L
RT: 4.692 min Scan# 1058
Delta R.T. 0.007 min
Lab File: VU062835.D
Acq: 16 Jan 2025 21:50




Instrument :
MSVOA_U
ClientSampleId :
BH8W9DL


Tgt Ion: 43 Resp: 10585
Ion Ratio Lower Upper
43 100
72 36.2 17.1 51.2

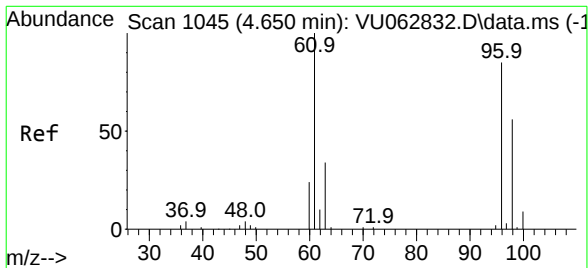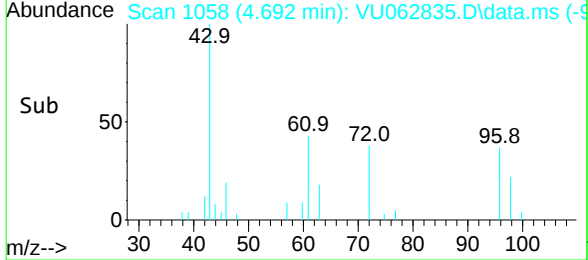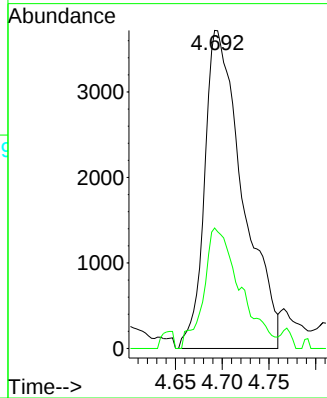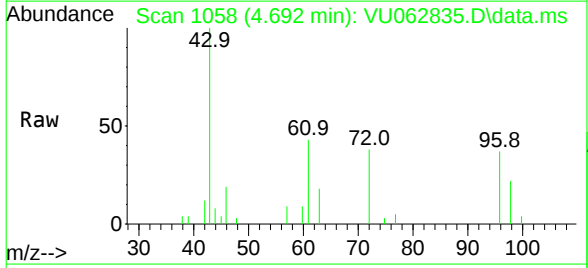

#22
cis-1,2-Dichloroethene
Concen: 5.048 ug/L
RT: 4.650 min Scan# 1045
Delta R.T. 0.000 min
Lab File: VU062835.D
Acq: 16 Jan 2025 21:50


Tgt Ion: 96 Resp: 40704
Ion Ratio Lower Upper
96 100
61 122.2 84.8 157.6
98 64.3 43.1 80.1

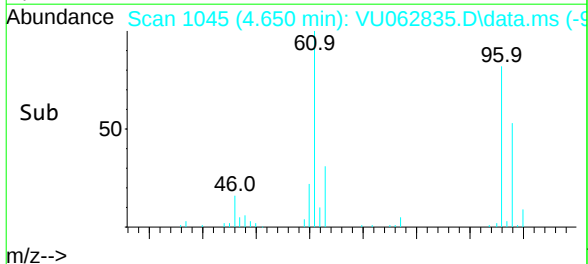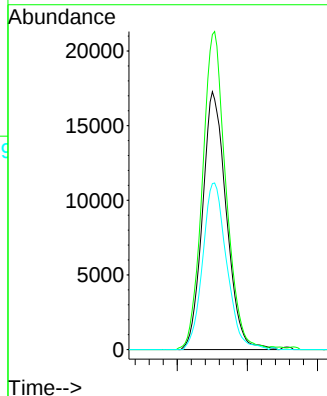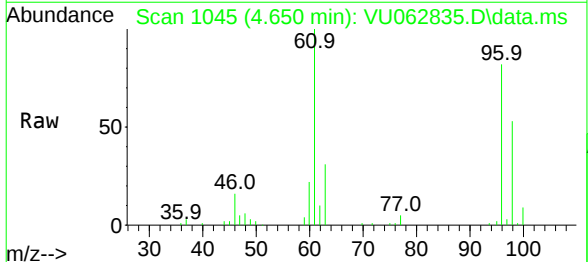

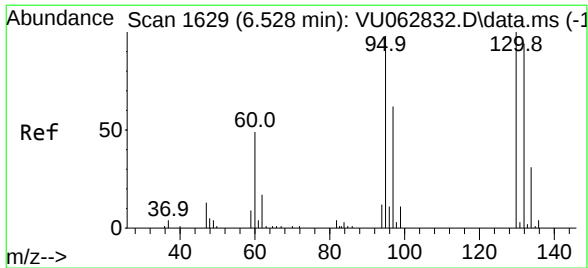

#34
 Trichloroethene
 Concen: 1.187 ug/L
 RT: 6.531 min Scan# 16
 Delta R.T. 0.003 min
 Lab File: VU062835.D
 Acq: 16 Jan 2025 21:50

Instrument :
 MSVOA_U
 ClientSampleId :
 BH8W9DL

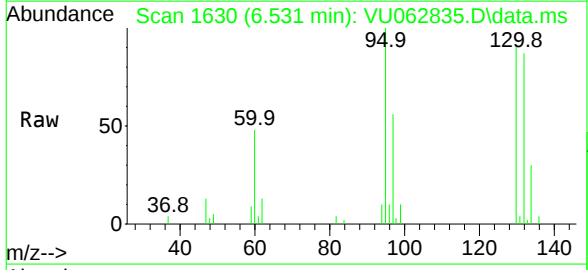

Tgt Ion:	95	Resp:	11943
Ion	Ratio	Lower	Upper
95	100		
97	55.6	47.5	88.3
132	86.7	66.9	124.3
130	91.4	68.6	127.4

